

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110121\
Data File : FF009232.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2021 16:01
Operator : AJ\MA
Sample : M4427-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FDR-BH-6-20211029-7.5-8

Integration File: autoint1.e
Quant Time: Nov 02 01:11:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.708	1364149	12.440 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110121\
Data File : FF009232.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2021 16:01
Operator : AJ\MA
Sample : M4427-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FDR-BH-6-20211029-7.5-8

Integration File: autoint1.e
Quant Time: Nov 02 01:11:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

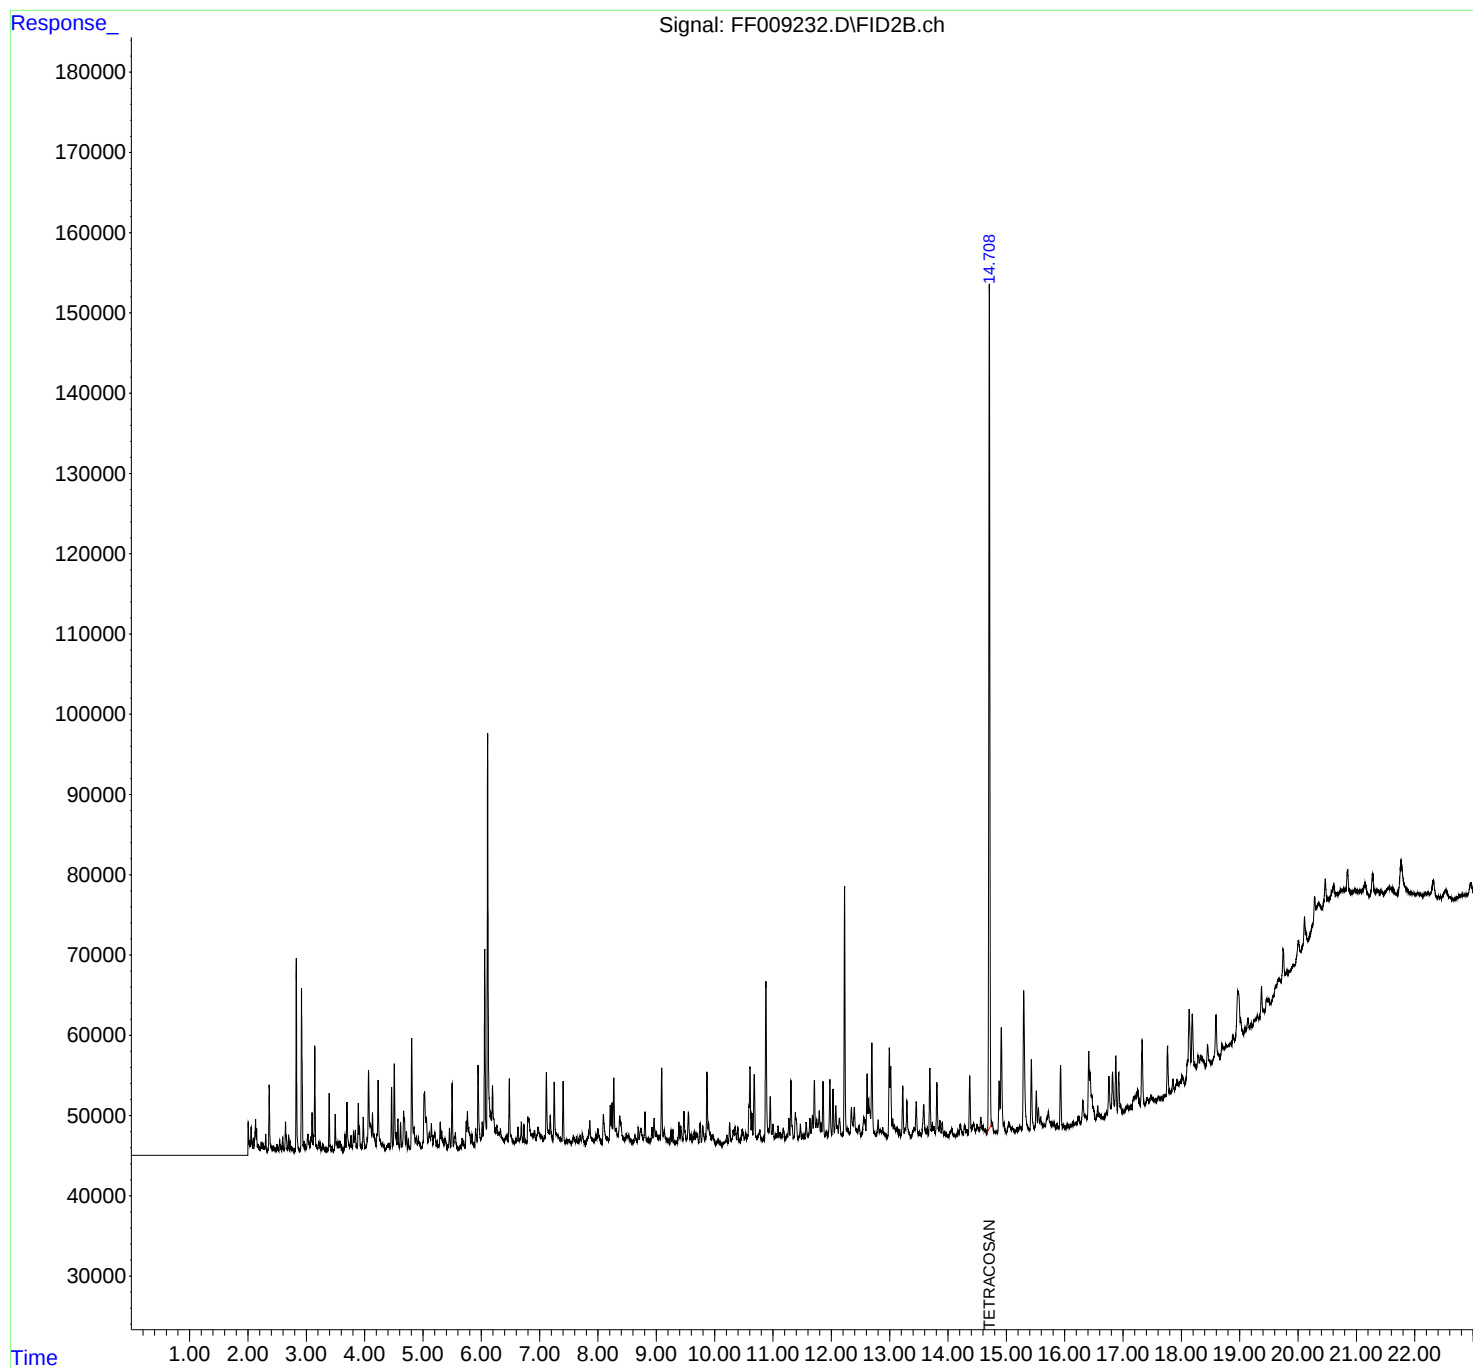

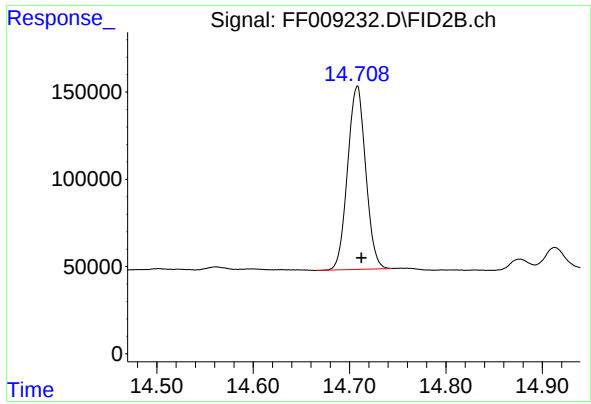

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.708 min
Delta R.T.: -0.004 min
Response: 1364149
Conc: 12.44 ug/ml

Instrument :
FID_F
ClientSampleId :
FDR-BH-6-20211029-7.5-8