

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110123\
Data File : FF 50X.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2023 15:30
Operator : YP\AJ
Sample : 05047-14 50X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 01 23:43:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.518	616824	5.038 ug/ml
3) N-DODECANE	6.683	984293	7.835 ug/ml
4) N-TETRADECANE	8.509	1032678	8.206 ug/ml
5) N-HEXADECANE	10.115	932828	7.253 ug/ml
6) N-OCTADECANE	11.556	747475	5.703 ug/ml
7) N-EICOSANE	12.867	380907	2.860 ug/ml
8) N-DOCOSANE	14.065	167110	1.270 ug/ml
10) N-TETRACOSANE	15.169	54698	0.415 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110123\
Data File : FF 50X.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2023 15:30
Operator : YP\AJ
Sample : 05047-14 50X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 01 23:43:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

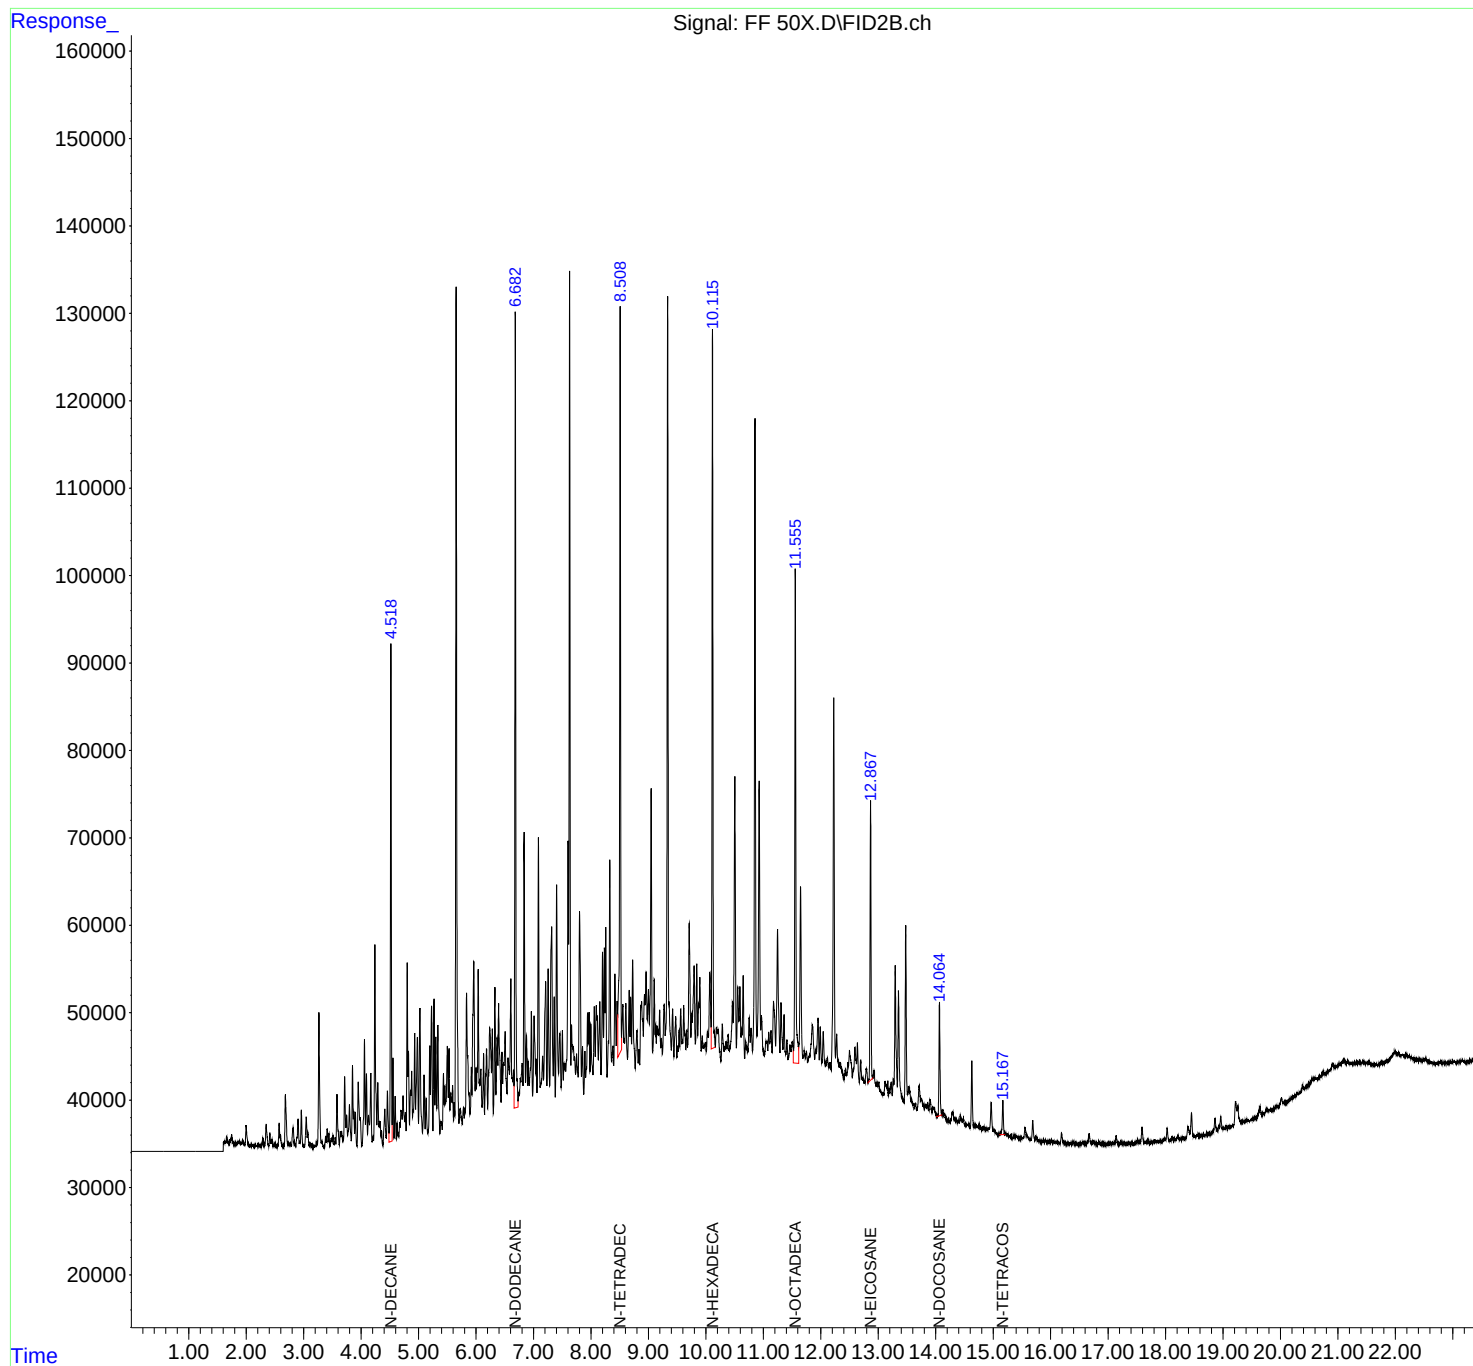


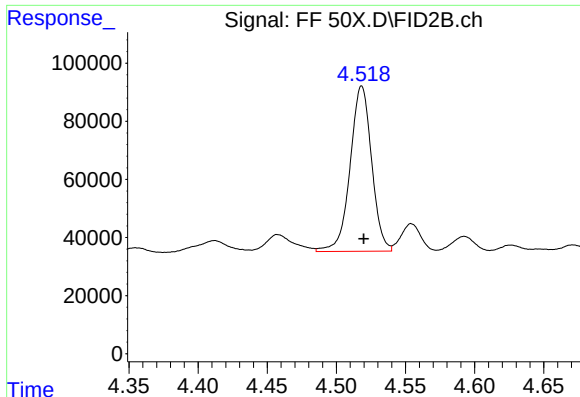

#2 N-DECANE


R.T.: 4.518 min
Delta R.T.: -0.001 min
Response: 616824
Conc: 5.04 ug/ml

Instrument :
FID_F
ClientSampleId :

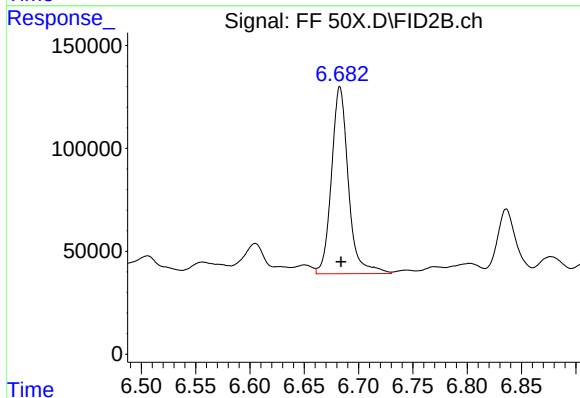


#3 N-DODECANE

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 984293
Conc: 7.84 ug/ml

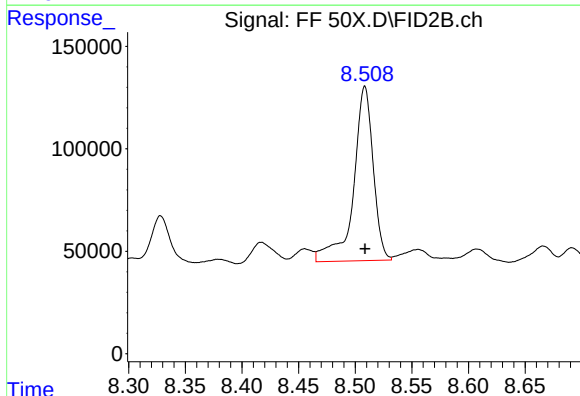


#4 N-TETRADECANE

R.T.: 8.509 min
Delta R.T.: 0.000 min
Response: 1032678
Conc: 8.21 ug/ml

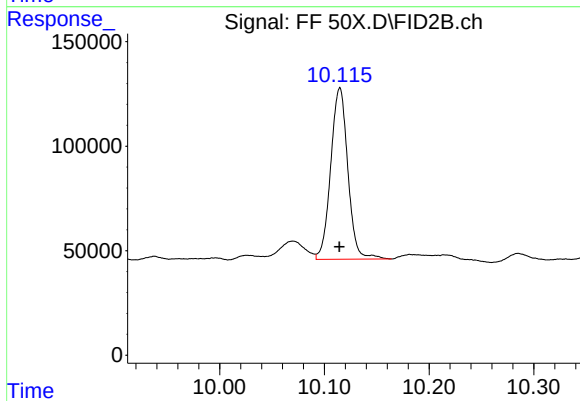

#5 N-HEXADECANE


R.T.: 10.115 min
Delta R.T.: 0.000 min
Response: 932828
Conc: 7.25 ug/ml

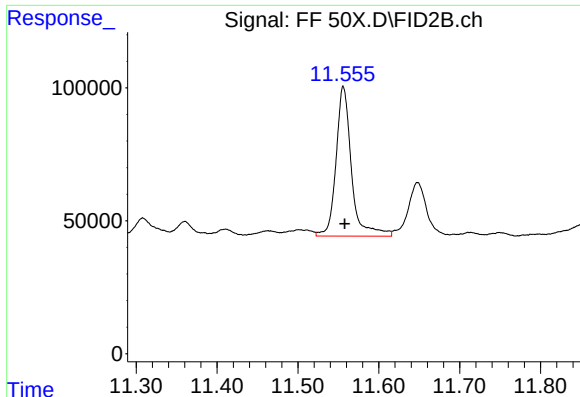

#6 N-OCTADECANE


R.T.: 11.556 min
Delta R.T.: -0.002 min
Response: 747475
Conc: 5.70 ug/ml

Instrument :
FID_F
ClientSampleId :

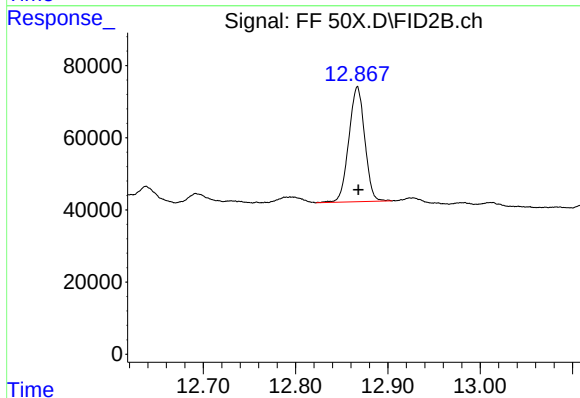


#7 N-EICOSANE

R.T.: 12.867 min
Delta R.T.: -0.001 min
Response: 380907
Conc: 2.86 ug/ml

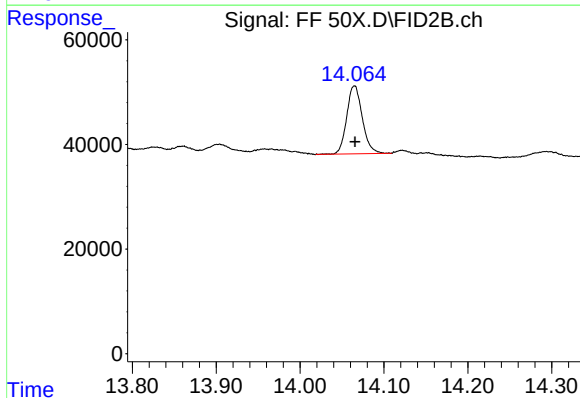


#8 N-DOCOSANE

R.T.: 14.065 min
Delta R.T.: 0.000 min
Response: 167110
Conc: 1.27 ug/ml

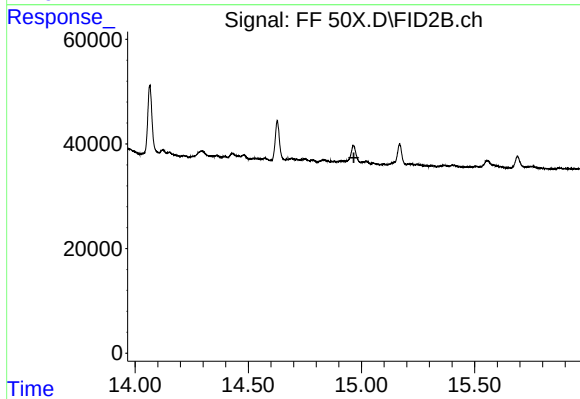

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.966 min
Response: 0
Conc: N.D.

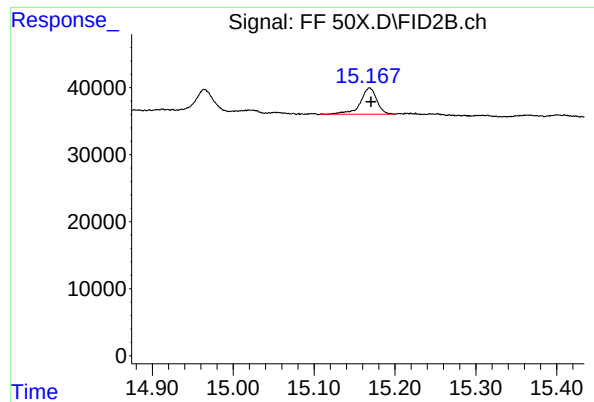

#10 N-TETRACOSANE

R.T.: 15.169 min
Delta R.T.: -0.002 min
Response: 54698
Conc: 0.41 ug/ml

Instrument :

FID_F

ClientSampleId :