

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009246.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 09:11
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:24:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.424	51968	0.532 ug/ml
16) N-HEXATRIACONTANE	20.123	396733	4.462 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009246.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 09:11
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:24:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

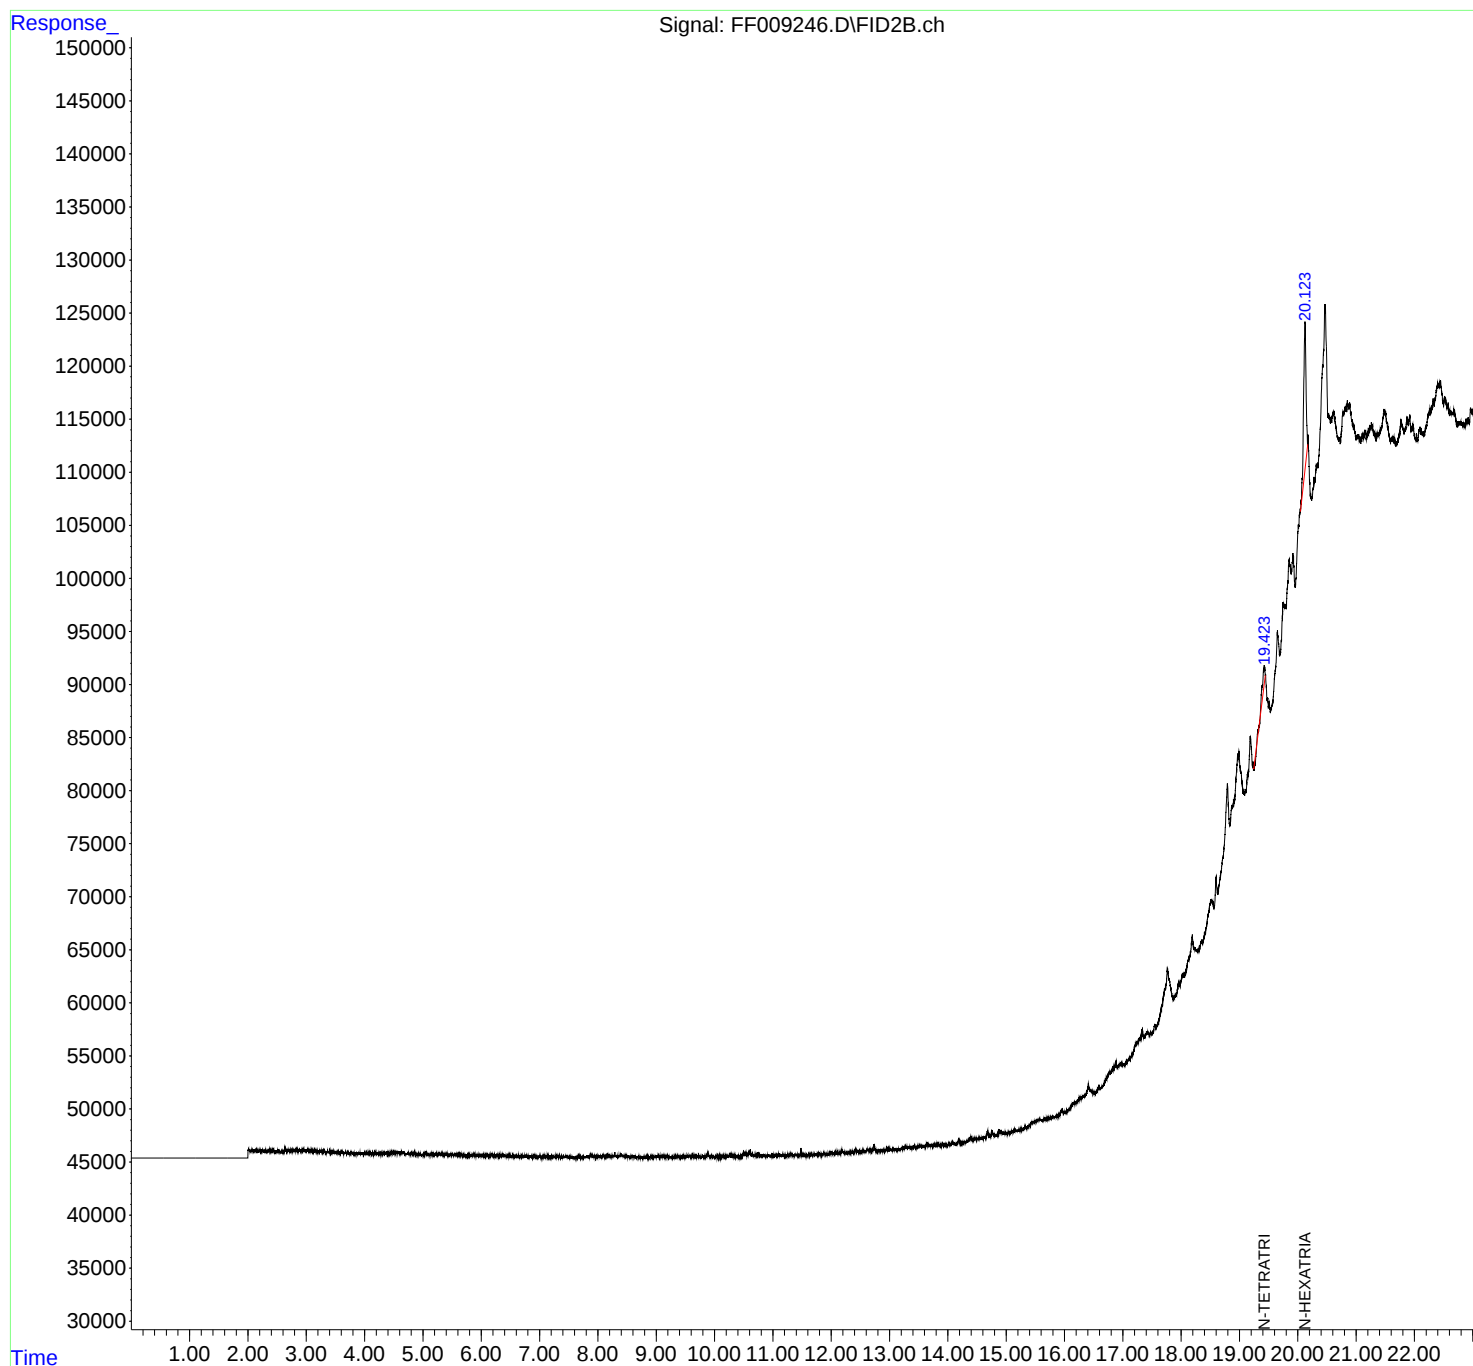


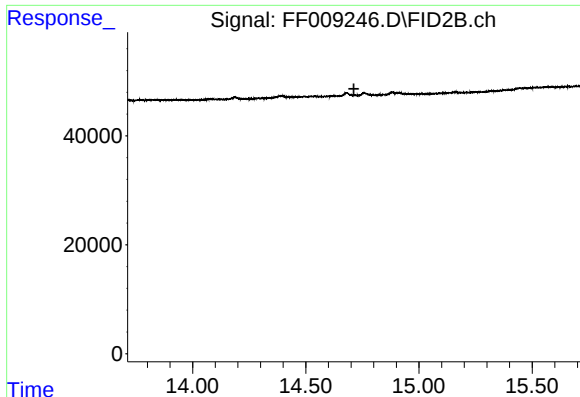

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.712 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

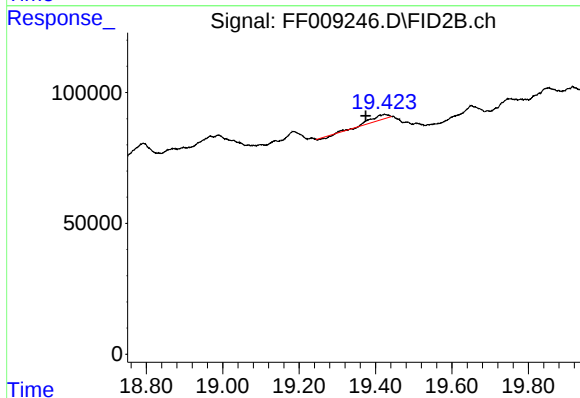

#15 N-TETRATRIACONTANE

R.T.: 19.424 min
Delta R.T.: 0.049 min
Response: 51968
Conc: 0.53 ug/ml

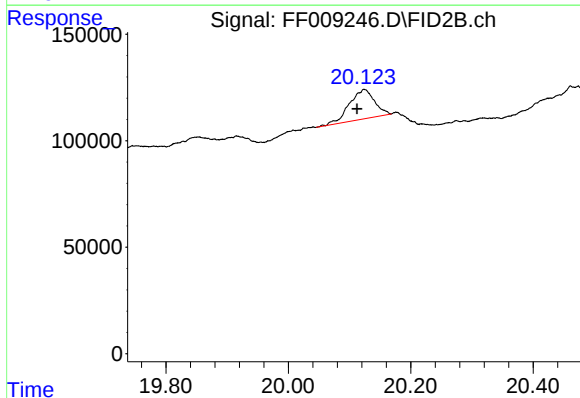

#16 N-HEXATRIACONTANE

R.T.: 20.123 min
Delta R.T.: 0.011 min
Response: 396733
Conc: 4.46 ug/ml