

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009249.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 10:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:25:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.478	2059774	16.213 ug/ml
12)	N-OCTACOSANE	16.879	2178137	18.607 ug/ml
13)	N-TRIACONTANE	17.764	90304	0.800 ug/ml
14)	N-DOTRIACONTANE	18.594	130972	1.240 ug/ml
15)	N-TETRATRIACONTANE	19.374	120349	1.231 ug/ml
16)	N-HEXATRIACONTANE	20.114	59156	0.665 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009249.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 10:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:25:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

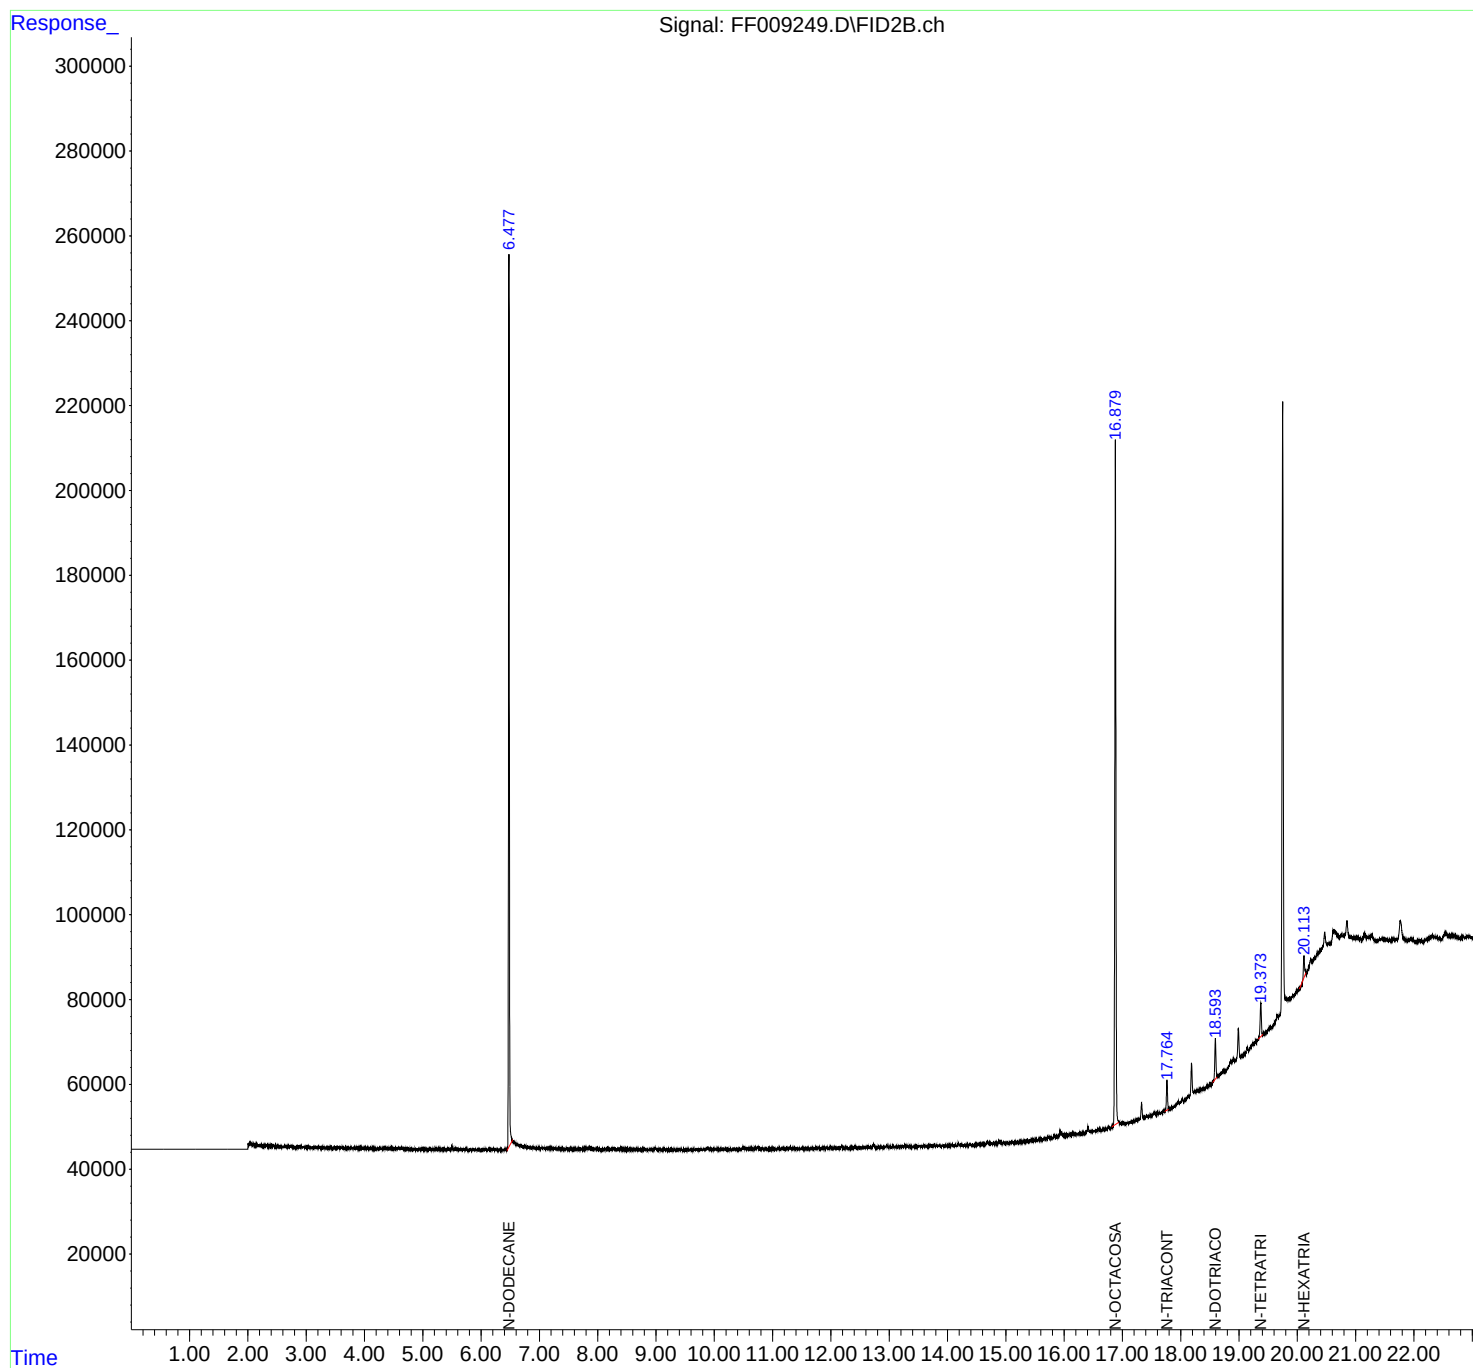


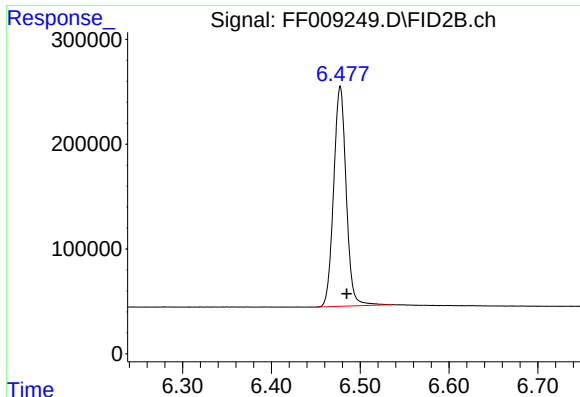

#3 N-DODECANE


R.T.: 6.478 min
Delta R.T.: -0.007 min
Response: 2059774
Conc: 16.21 ug/ml

Instrument :
FID_F
ClientSampleId :

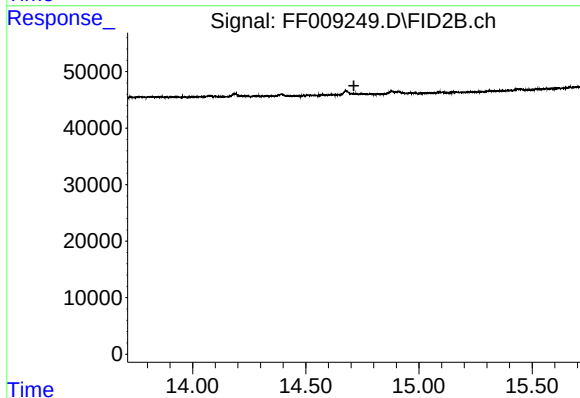


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

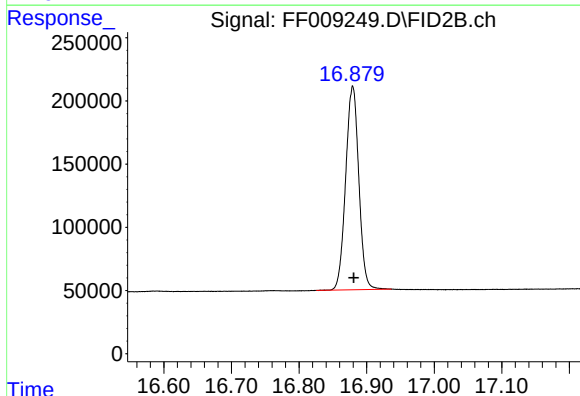


#12 N-OCTACOSANE

R.T.: 16.879 min
Delta R.T.: -0.001 min
Response: 2178137
Conc: 18.61 ug/ml

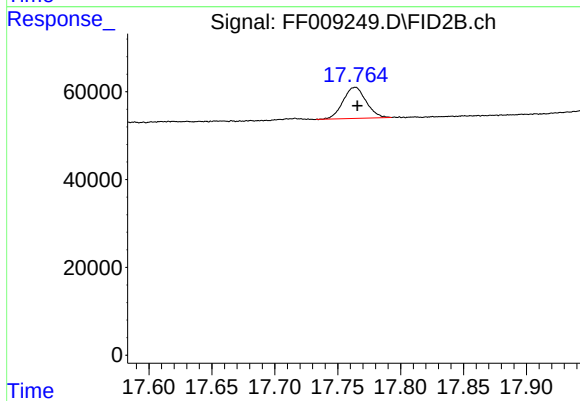

#13 N-TRIACONTANE


R.T.: 17.764 min
Delta R.T.: -0.001 min
Response: 90304
Conc: 0.80 ug/ml

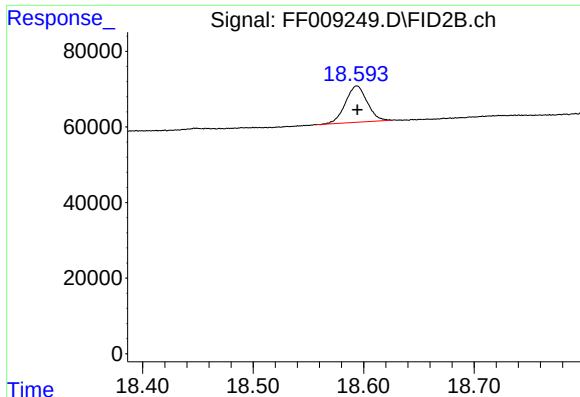

#14 N-DOTRIACONTANE


R.T.: 18.594 min
Delta R.T.: 0.000 min
Response: 130972
Conc: 1.24 ug/ml

Instrument :
FID_F
ClientSampleId :

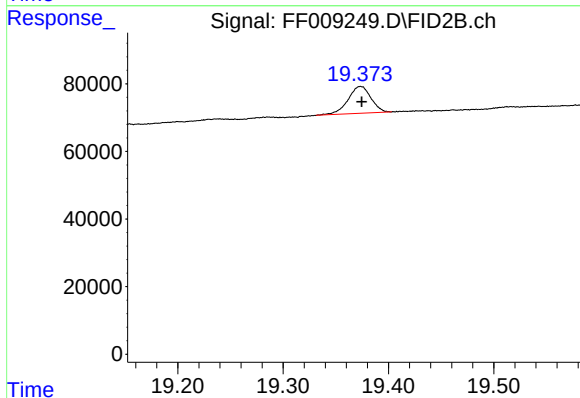

#15 N-TETRATRIACONTANE

R.T.: 19.374 min
Delta R.T.: 0.000 min
Response: 120349
Conc: 1.23 ug/ml

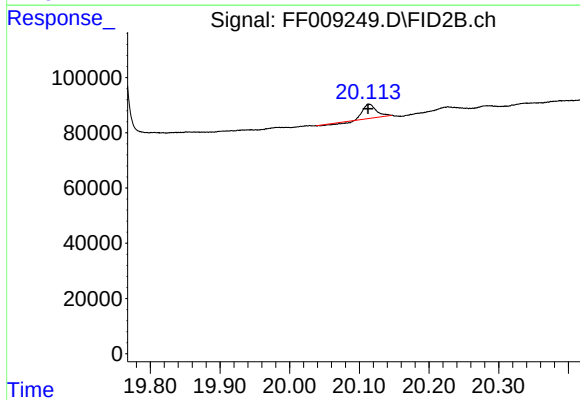

#16 N-HEXATRIACONTANE

R.T.: 20.114 min
Delta R.T.: 0.002 min
Response: 59156
Conc: 0.67 ug/ml