

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF110221\  
Data File : FF009251.D  
Signal(s) : FID2B.ch  
Acq On : 02 Nov 2021 11:50  
Operator : AJ\MA  
Sample : M4427-02 200X  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 03 01:26:30 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100721.M  
Quant Title :  
QLast Update : Fri Oct 08 02:25:33 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.    | Response | Conc Units  |
|-----------------------------|---------|----------|-------------|
| -----                       |         |          |             |
| System Monitoring Compounds |         |          |             |
| Target Compounds            |         |          |             |
| 5) N-HEXADECANE             | 9.869   | 268741   | 2.117 ug/ml |
| 6) N-OCTADECANE             | 11.305  | 276174   | 2.142 ug/ml |
| 7) N-EICOSANE               | 12.656  | 156351   | 1.215 ug/ml |
| 12) N-OCTACOSANE            | 16.818f | 138022   | 1.179 ug/ml |
| -----                       |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF110221\  
Data File : FF009251.D  
Signal(s) : FID2B.ch  
Acq On : 02 Nov 2021 11:50  
Operator : AJ\MA  
Sample : M4427-02 200X  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 03 01:26:30 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100721.M  
Quant Title :  
QLast Update : Fri Oct 08 02:25:33 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

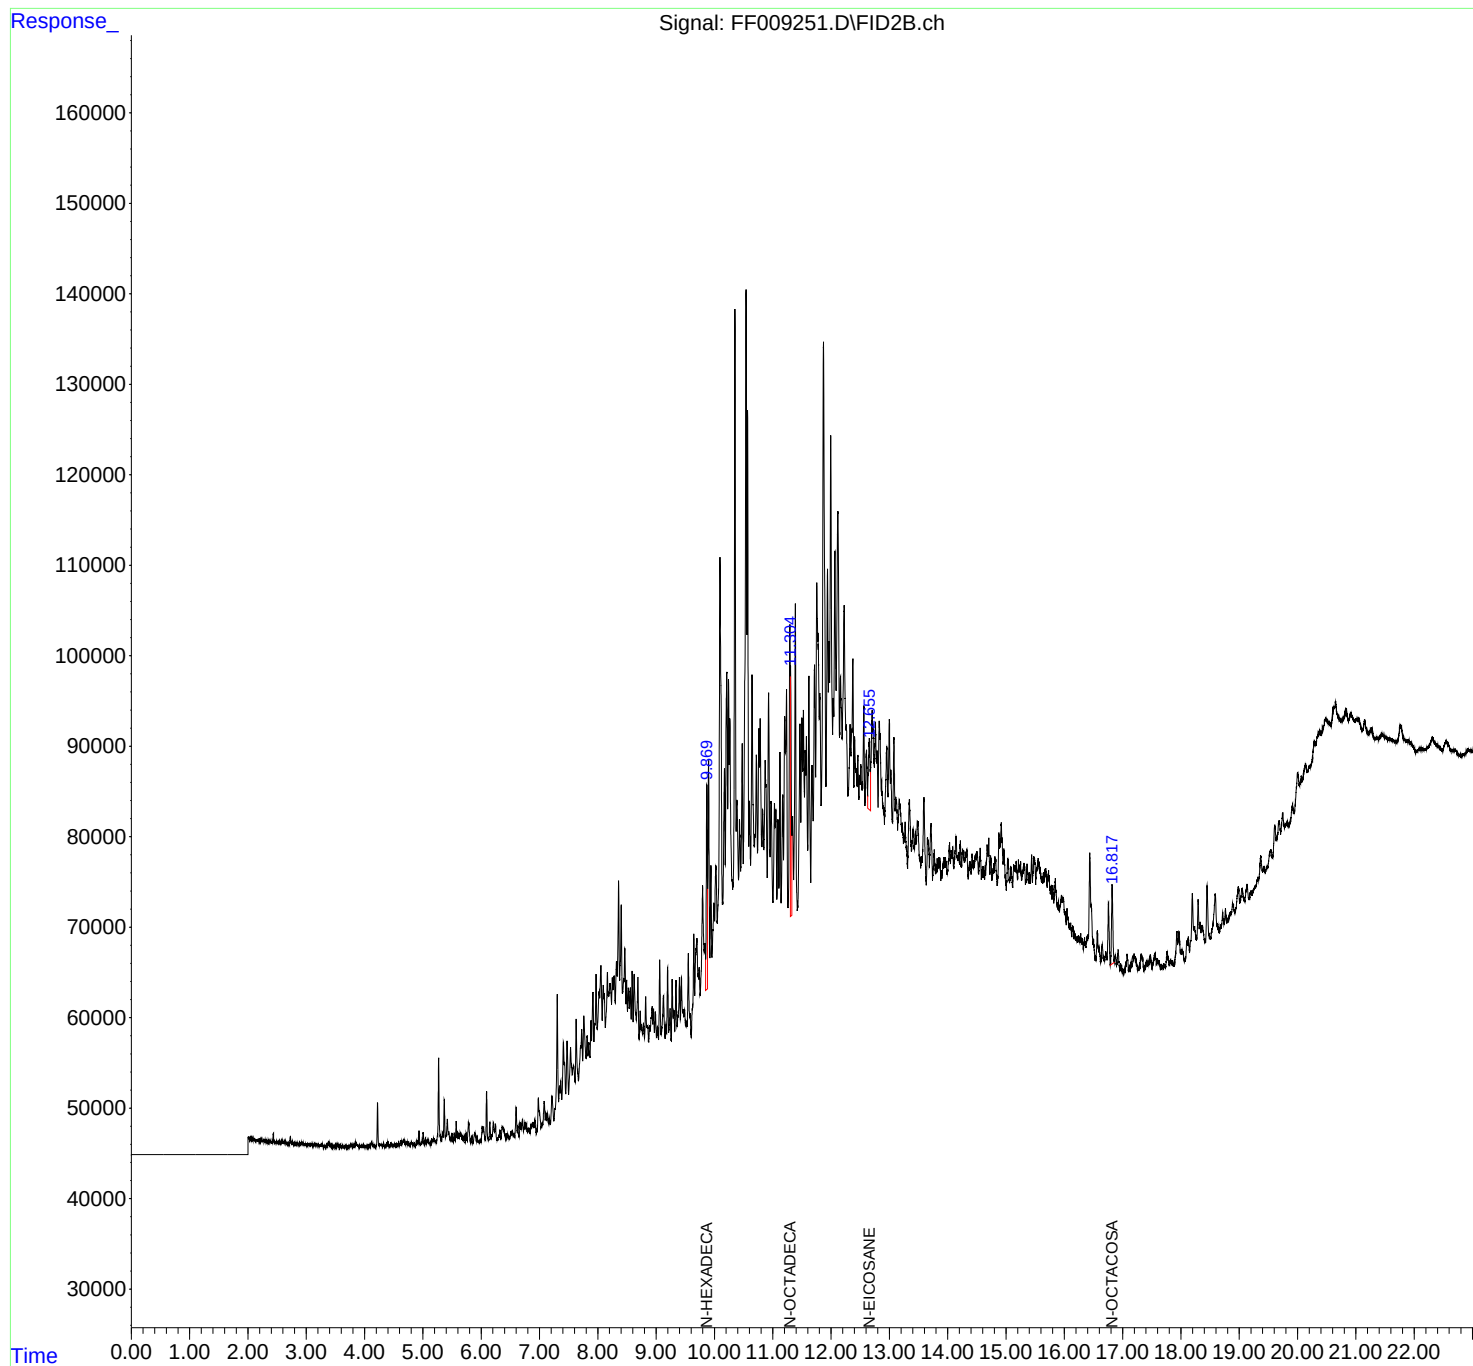


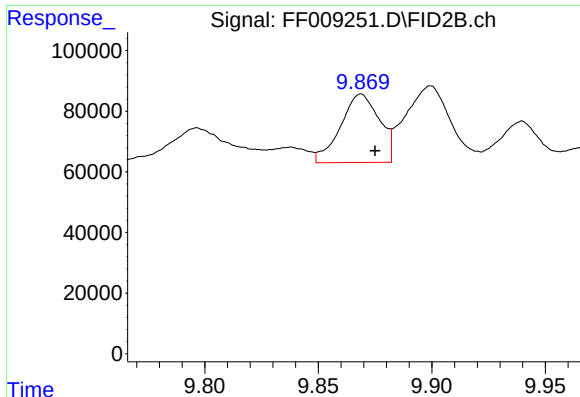

#5 N-HEXADECANE


R.T.: 9.869 min  
Delta R.T.: -0.006 min  
Response: 268741  
Conc: 2.12 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

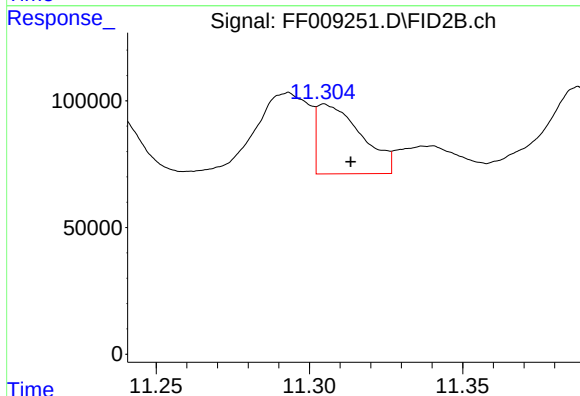


#6 N-OCTADECANE

R.T.: 11.305 min  
Delta R.T.: -0.009 min  
Response: 276174  
Conc: 2.14 ug/ml

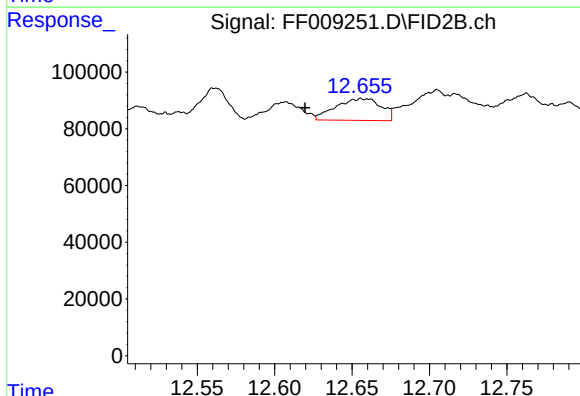


#7 N-EICOSANE

R.T.: 12.656 min  
Delta R.T.: 0.036 min  
Response: 156351  
Conc: 1.21 ug/ml

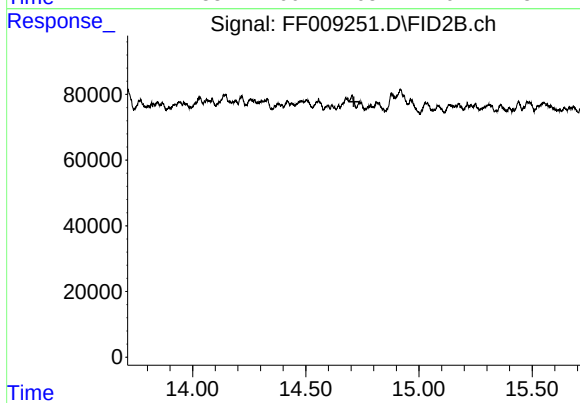

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.712 min  
Response: 0  
Conc: N.D.

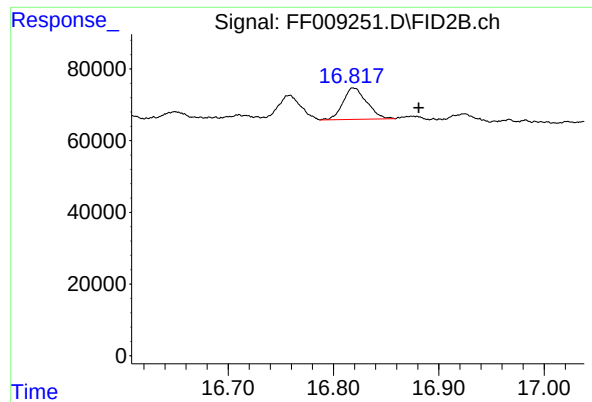

#12 N-OCTACOSANE

R.T.: 16.818 min  
Delta R.T.: -0.063 min  
Response: 138022  
Conc: 1.18 ug/ml

Instrument :

FID\_F

ClientSampleId :