

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009255.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 14:06
Operator : AJ\MA
Sample : M4427-06 100X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:27:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-HEXADECANE	9.868	74621	0.588 ug/ml
6) N-OCTADECANE	11.291	275491	2.137 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009255.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 14:06
Operator : AJ\MA
Sample : M4427-06 100X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:27:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

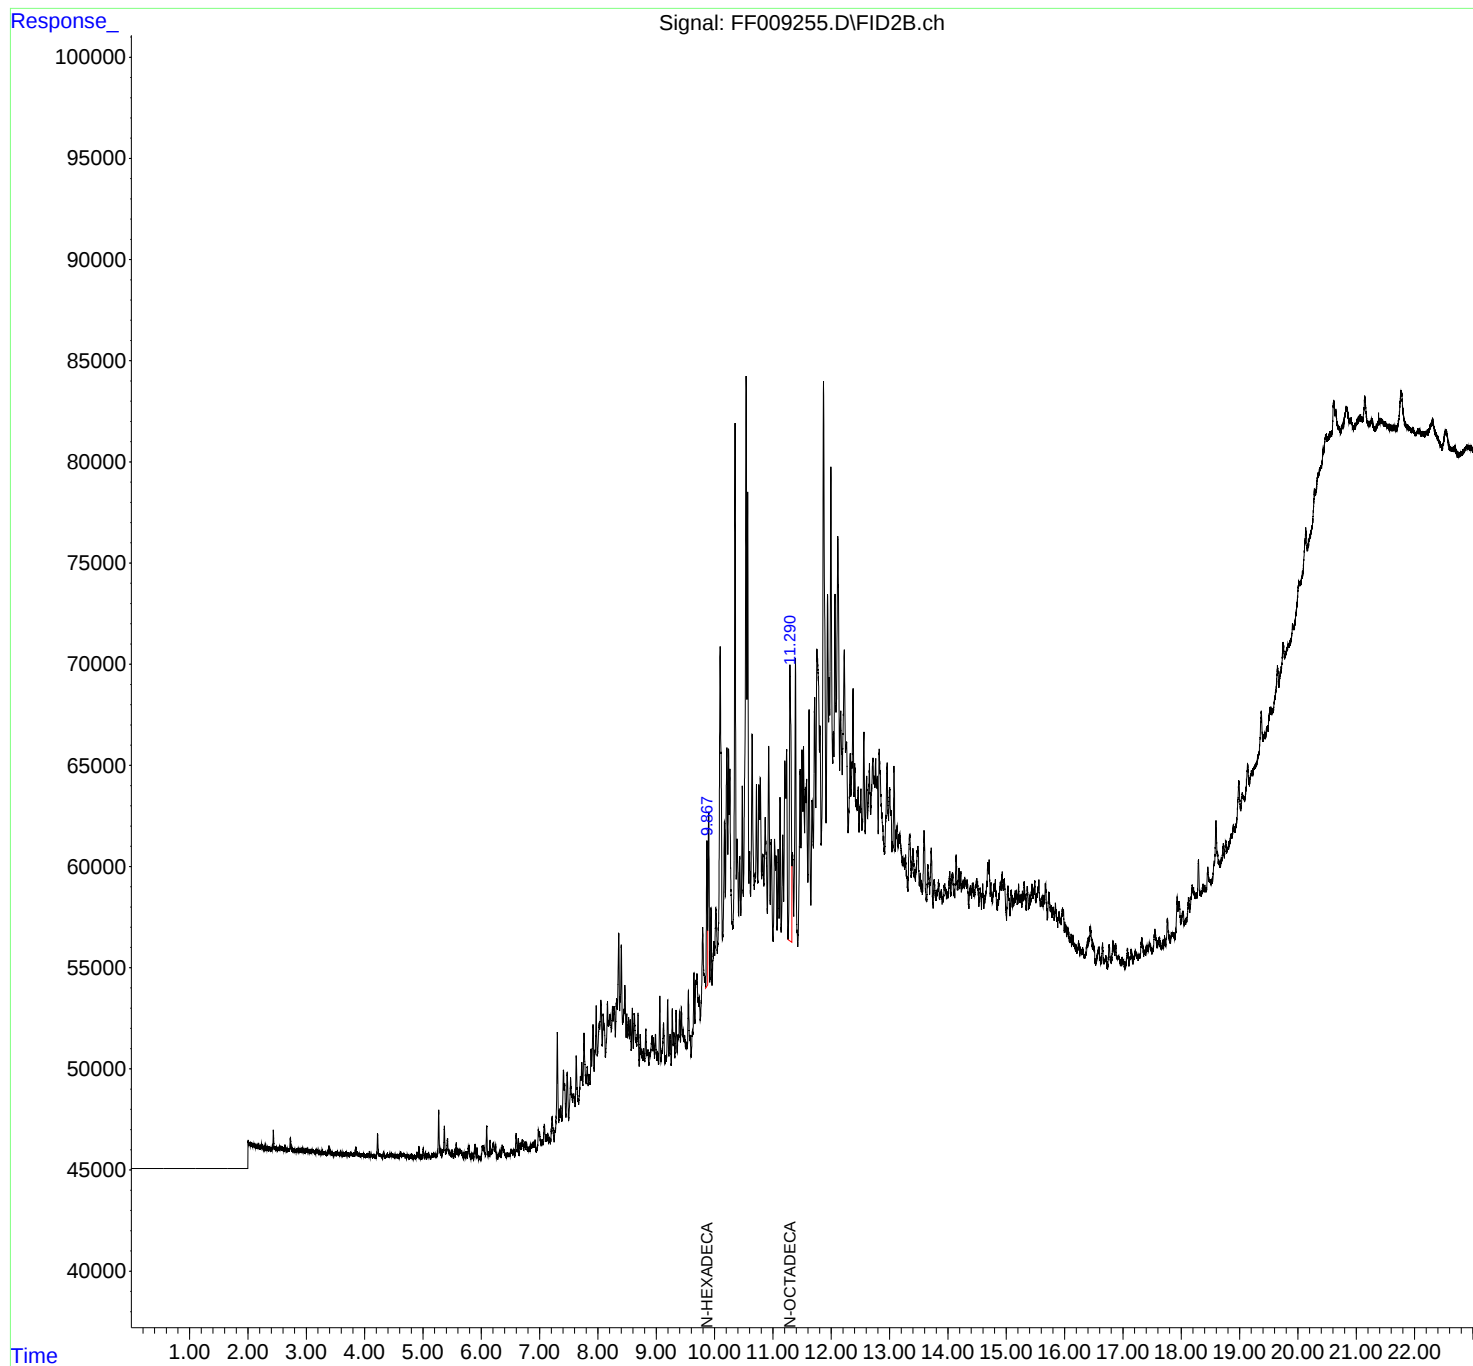


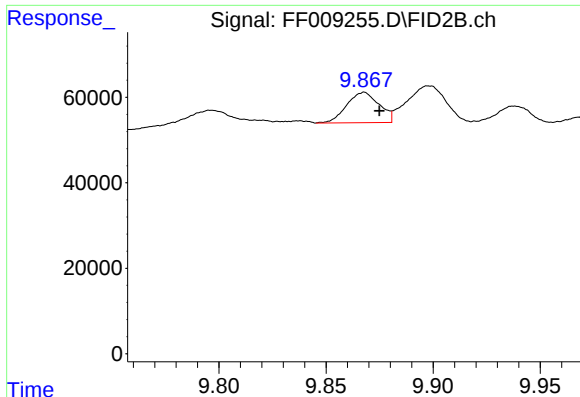

#5 N-HEXADECANE


R.T.: 9.868 min
Delta R.T.: -0.007 min
Response: 74621
Conc: 0.59 ug/ml

Instrument :
FID_F
ClientSampleId :

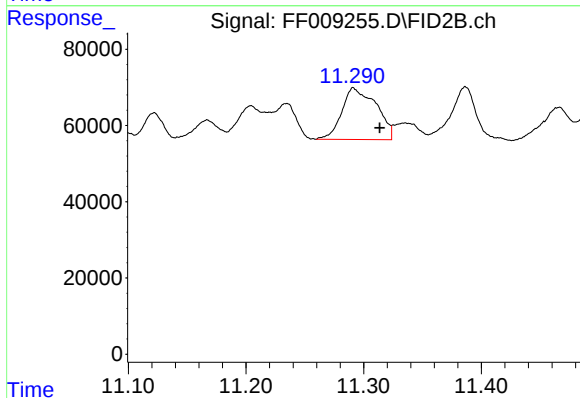

#6 N-OCTADECANE

R.T.: 11.291 min
Delta R.T.: -0.023 min
Response: 275491
Conc: 2.14 ug/ml

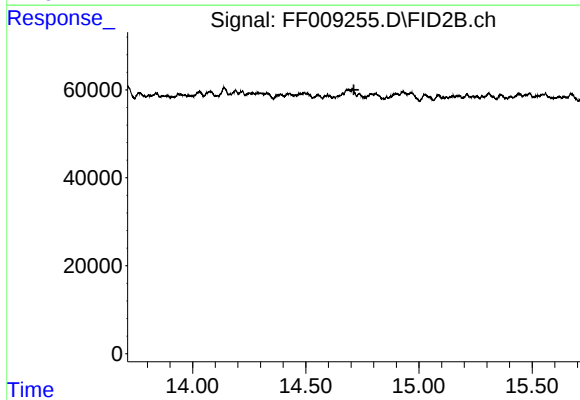

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.