

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009256.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 14:36
Operator : AJ\MA
Sample : M4427-07 50X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:27:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
5)	N-HEXADECANE	9.867	96831	0.763 ug/ml
6)	N-OCTADECANE	11.291	375676	2.914 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009256.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 14:36
Operator : AJ\MA
Sample : M4427-07 50X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:27:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

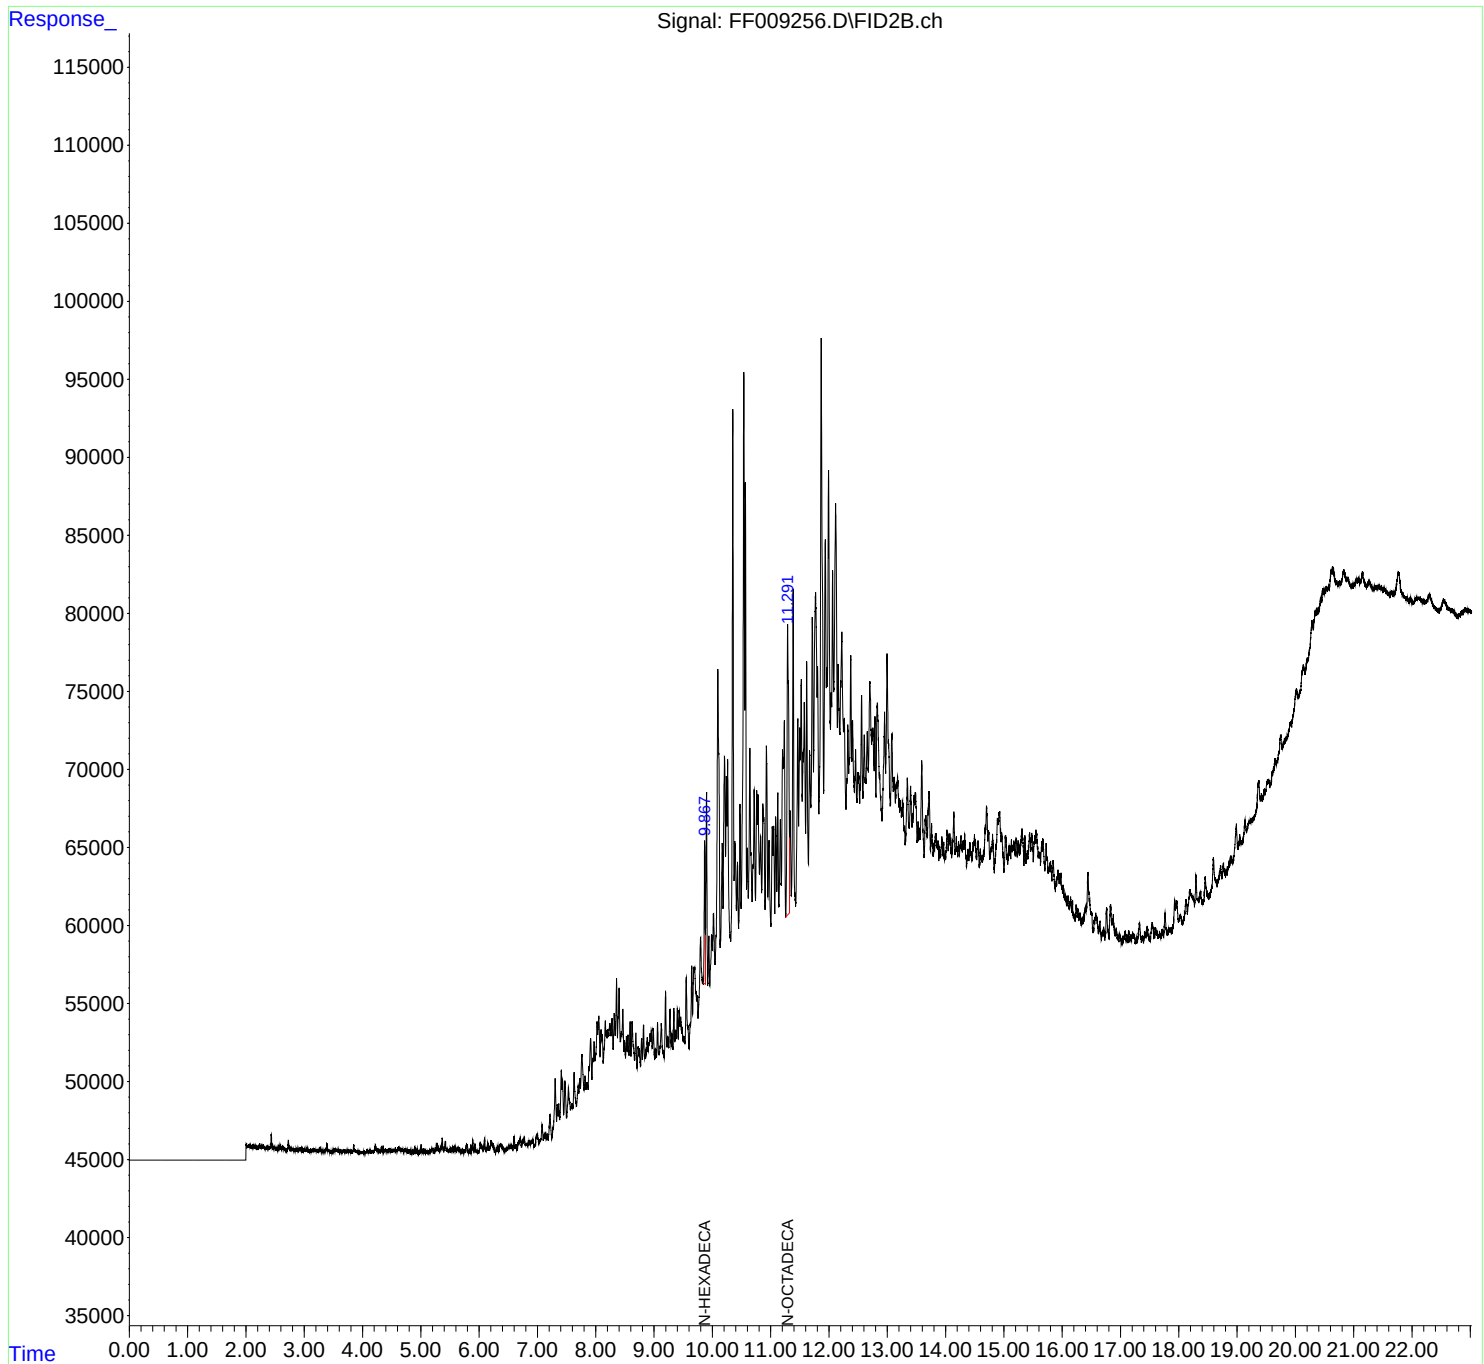


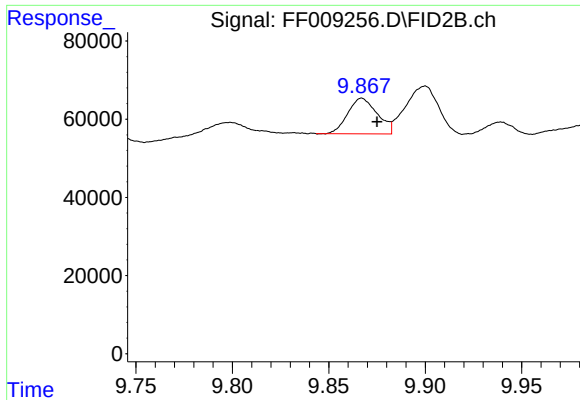

#5 N-HEXADECANE


R.T.: 9.867 min
Delta R.T.: -0.008 min
Response: 96831
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

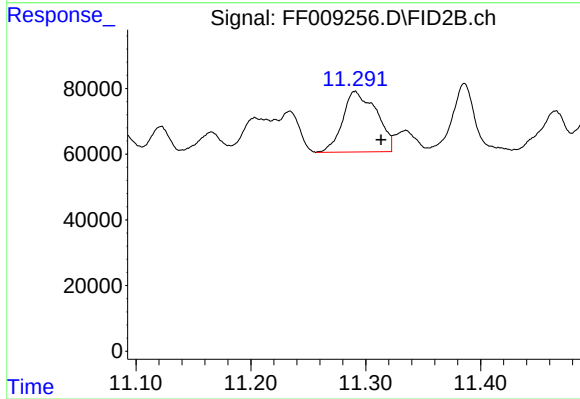

#6 N-OCTADECANE

R.T.: 11.291 min
Delta R.T.: -0.022 min
Response: 375676
Conc: 2.91 ug/ml

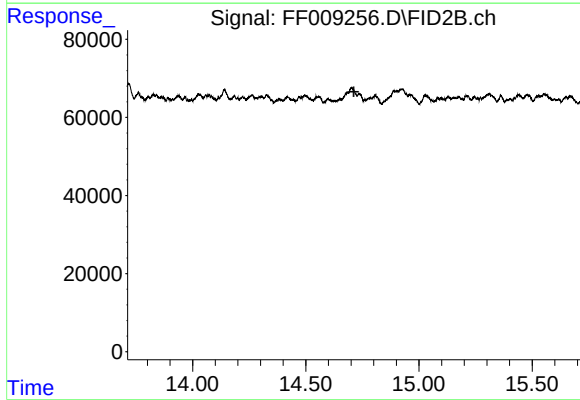

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.