

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009257.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 15:07
Operator : AJ\MA
Sample : M4427-08 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:28:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-HEXADECANE	9.868	115086	0.906 ug/ml
6) N-OCTADECANE	11.305	192291	1.492 ug/ml
7) N-EICOSANE	12.561f	119349	0.927 ug/ml
10) N-TETRACOSANE	14.912	213804	1.708 ug/ml
12) N-OCTACOSANE	16.816f	206258	1.762 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110221\
Data File : FF009257.D
Signal(s) : FID2B.ch
Acq On : 02 Nov 2021 15:07
Operator : AJ\MA
Sample : M4427-08 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:28:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

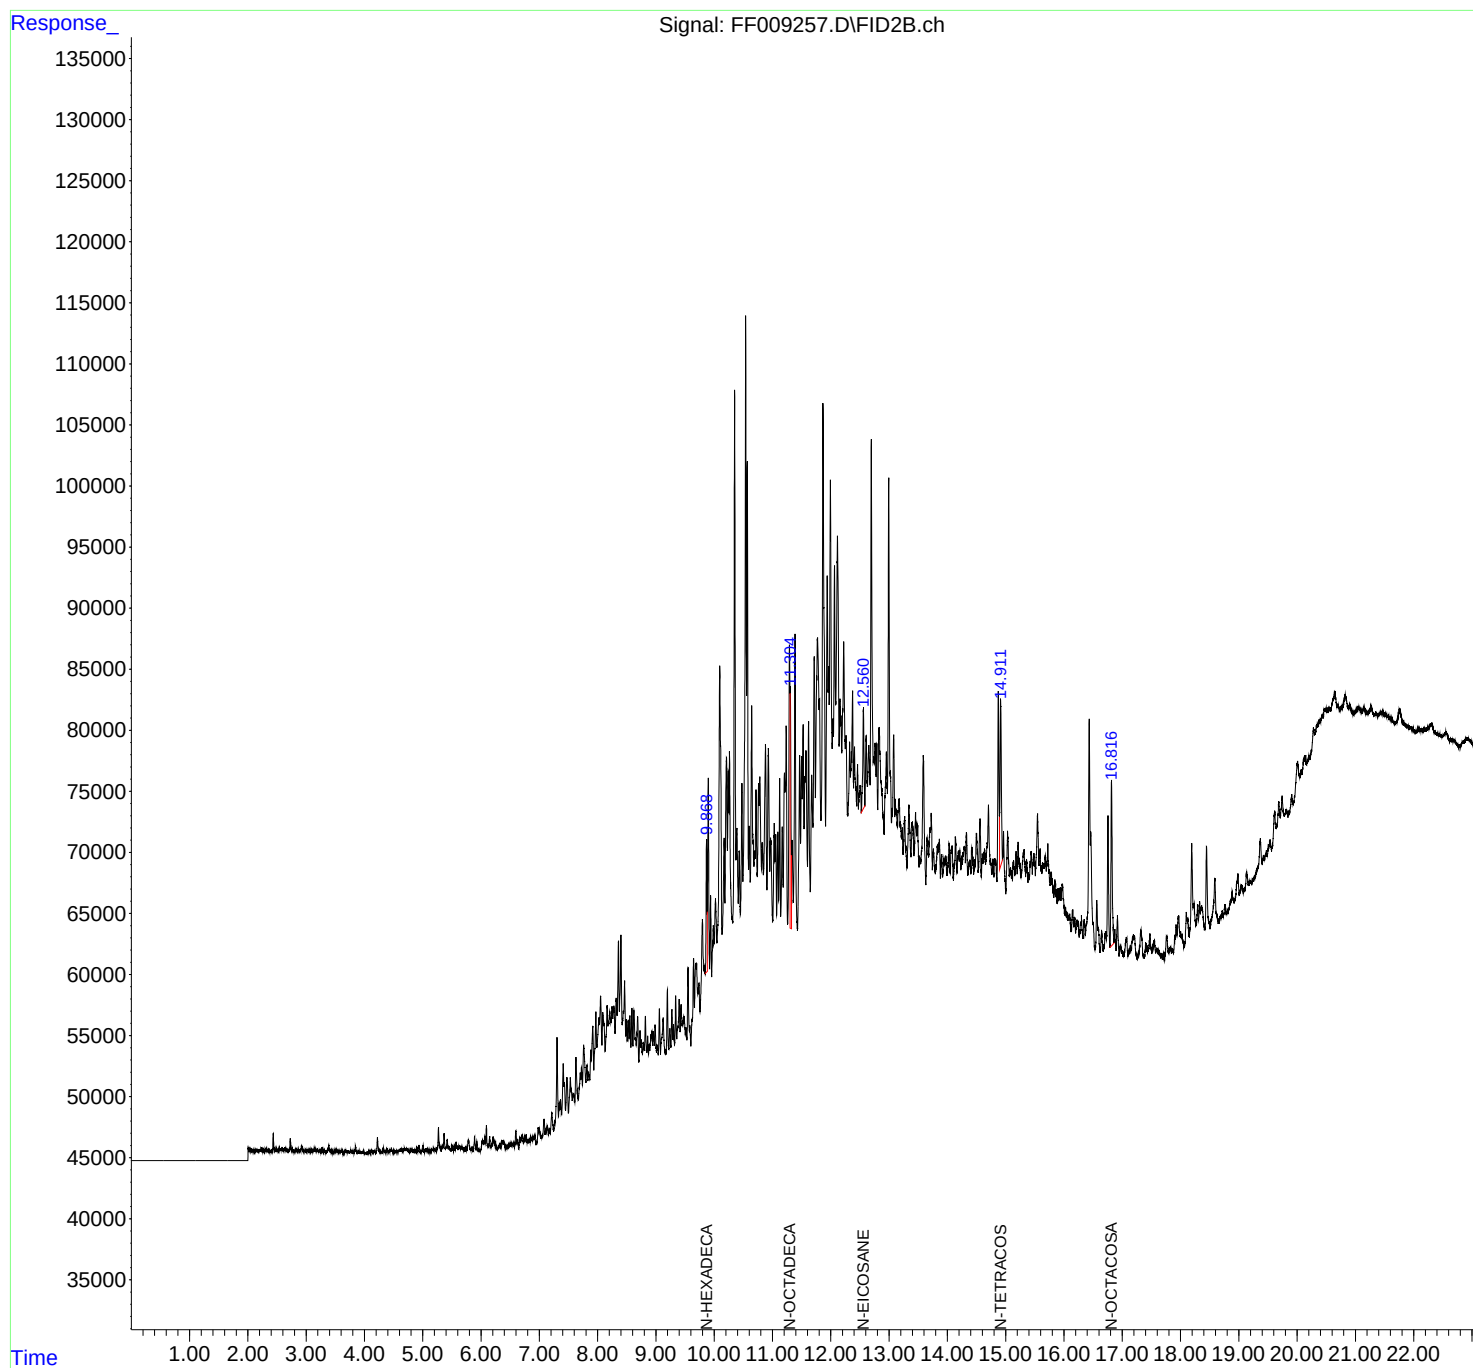


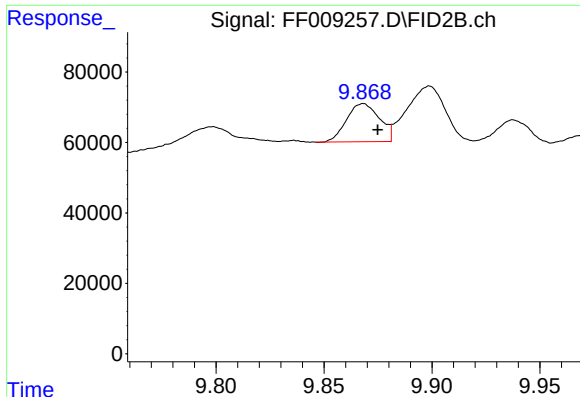

#5 N-HEXADECANE


R.T.: 9.868 min
Delta R.T.: -0.007 min
Response: 115086
Conc: 0.91 ug/ml

Instrument :
FID_F
ClientSampleId :

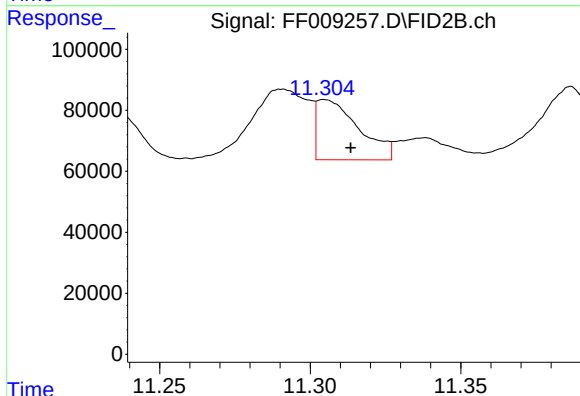


#6 N-OCTADECANE

R.T.: 11.305 min
Delta R.T.: -0.009 min
Response: 192291
Conc: 1.49 ug/ml

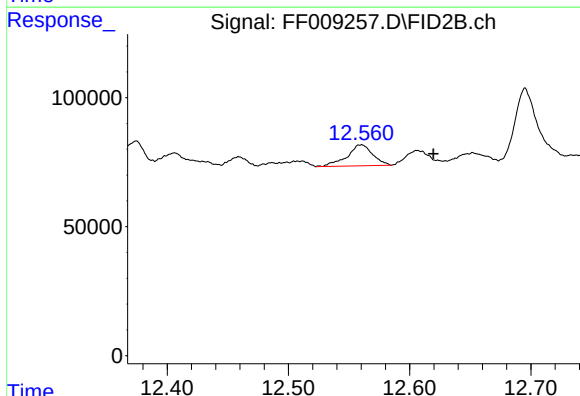


#7 N-EICOSANE

R.T.: 12.561 min
Delta R.T.: -0.059 min
Response: 119349
Conc: 0.93 ug/ml

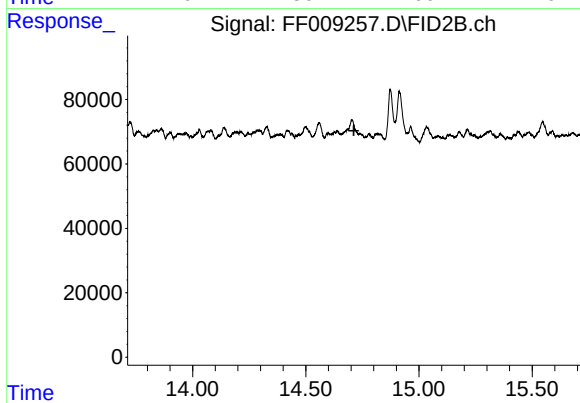

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

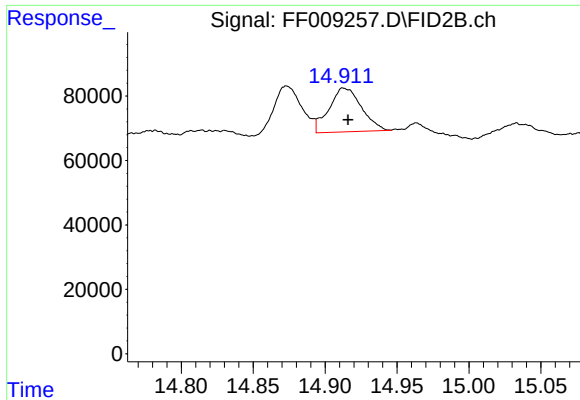

#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.004 min
Response: 213804
Conc: 1.71 ug/ml

Instrument :
FID_F
ClientSampleId :

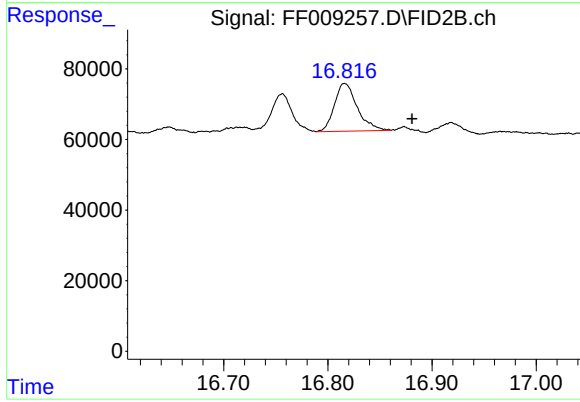

#12 N-OCTACOSANE

R.T.: 16.816 min
Delta R.T.: -0.065 min
Response: 206258
Conc: 1.76 ug/ml