

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110321\
 Data File : FF009270.D
 Signal(s) : FID2B.ch
 Acq On : 03 Nov 2021 09:51
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 03 12:08:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.709	1940115	17.693 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.765	98382	0.872 ug/ml
14) N-DOTRIACONTANE	18.594	115956	1.098 ug/ml
15) N-TETRATRIACONTANE	19.375	120078	1.229 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110321\
Data File : FF009270.D
Signal(s) : FID2B.ch
Acq On : 03 Nov 2021 09:51
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 12:08:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

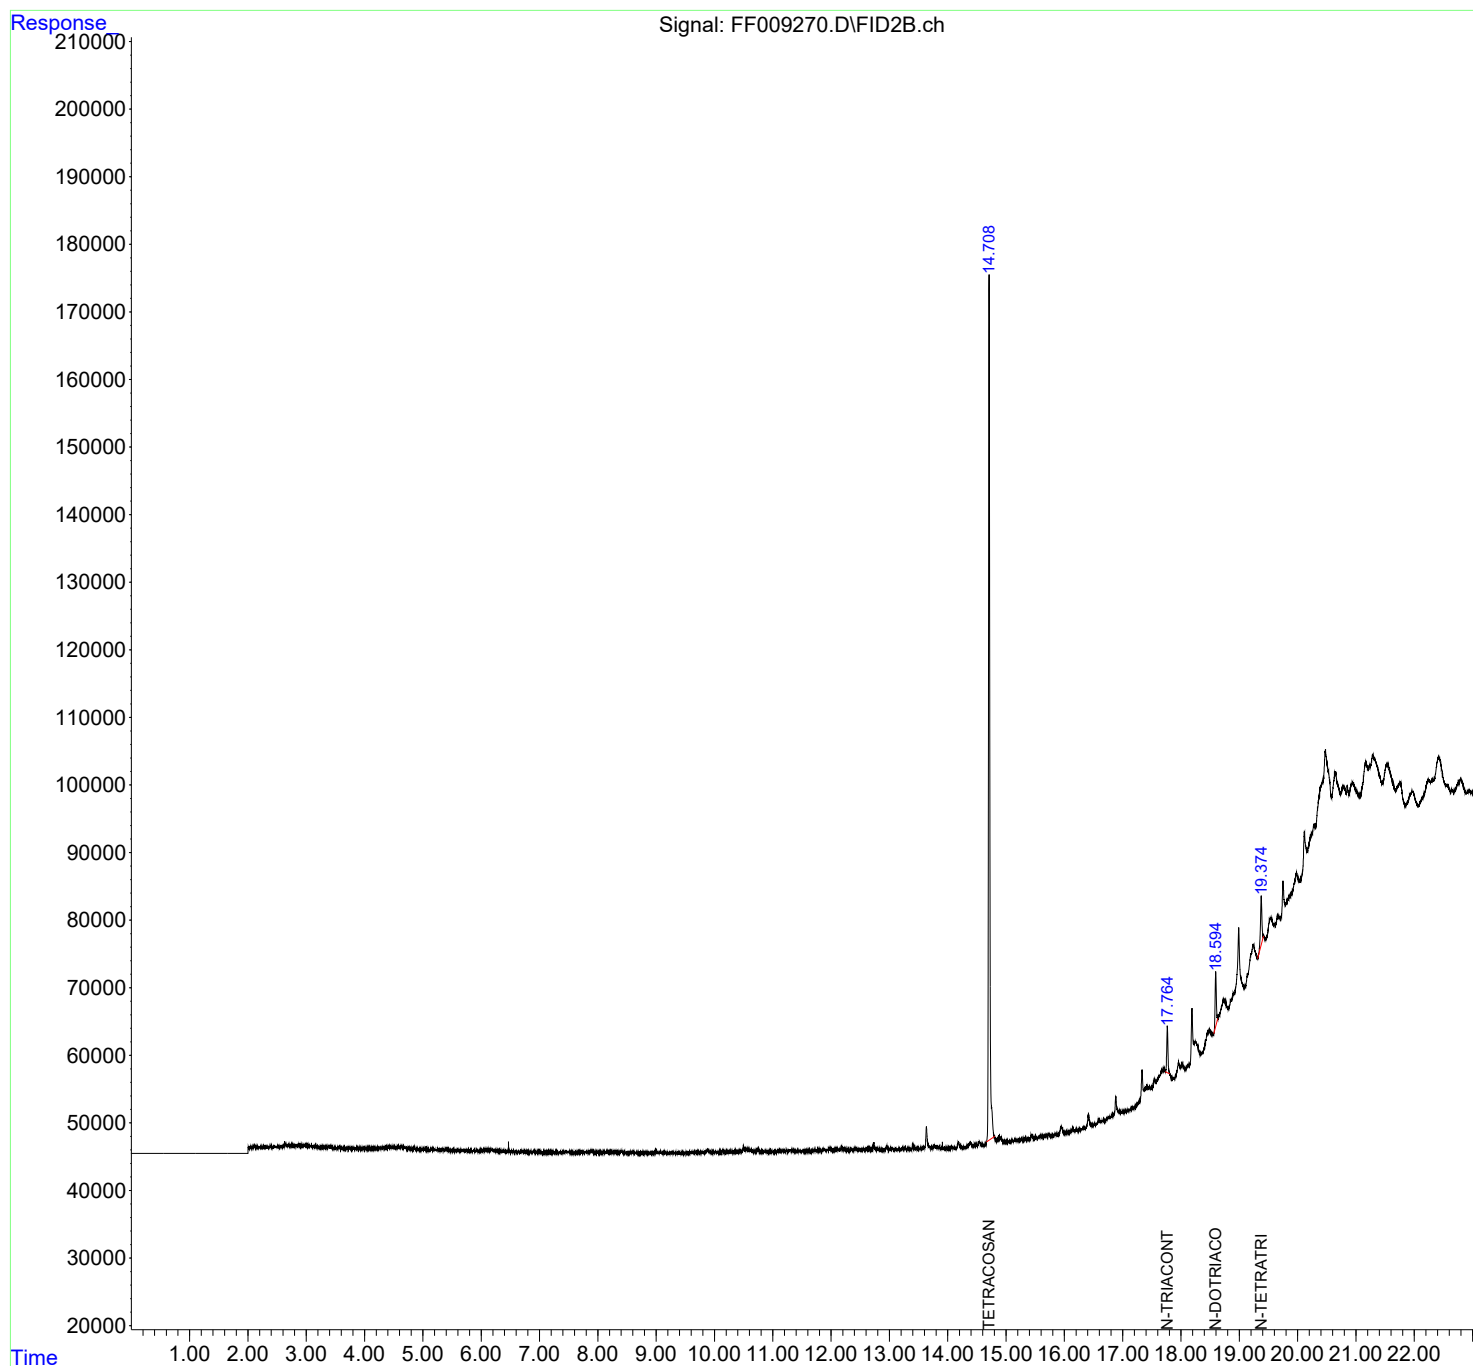


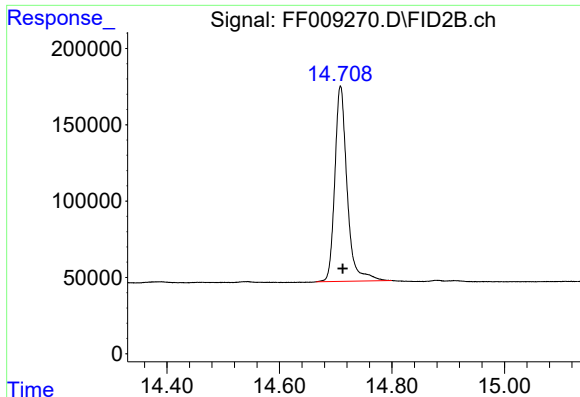

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.709 min
Delta R.T.: -0.004 min
Response: 1940115
Conc: 17.69 ug/ml

Instrument :
FID_F
ClientSampleId :

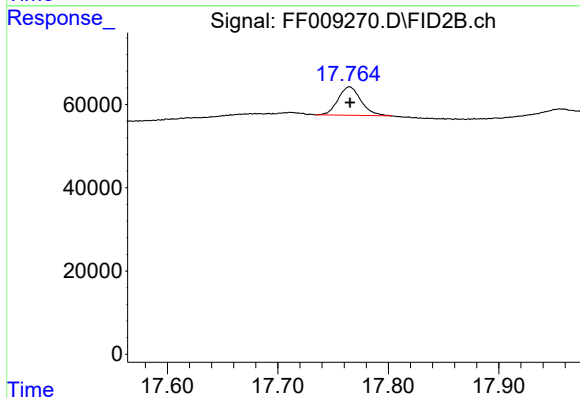


#13 N-TRIACONTANE

R.T.: 17.765 min
Delta R.T.: -0.001 min
Response: 98382
Conc: 0.87 ug/ml

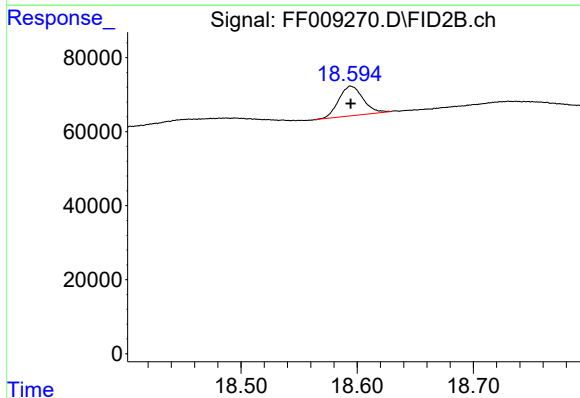

#14 N-DOTRIACONTANE

R.T.: 18.594 min
Delta R.T.: 0.000 min
Response: 115956
Conc: 1.10 ug/ml

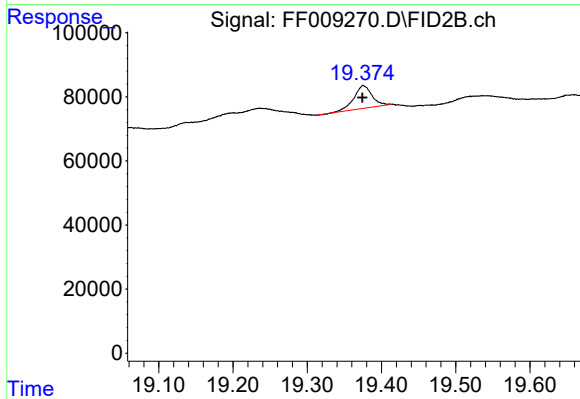

#15 N-TETRATRIACONTANE

R.T.: 19.375 min
Delta R.T.: 0.000 min
Response: 120078
Conc: 1.23 ug/ml