

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110321\
Data File : FF009273.D
Signal(s) : FID2B.ch
Acq On : 03 Nov 2021 11:24
Operator : AJ\MA
Sample : M4438-02 400X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 14:56:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-HEXADECANE	9.868	114122	0.899 ug/ml
6) N-OCTADECANE	11.291	427077	3.313 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110321\
Data File : FF009273.D
Signal(s) : FID2B.ch
Acq On : 03 Nov 2021 11:24
Operator : AJ\MA
Sample : M4438-02 400X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 14:56:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

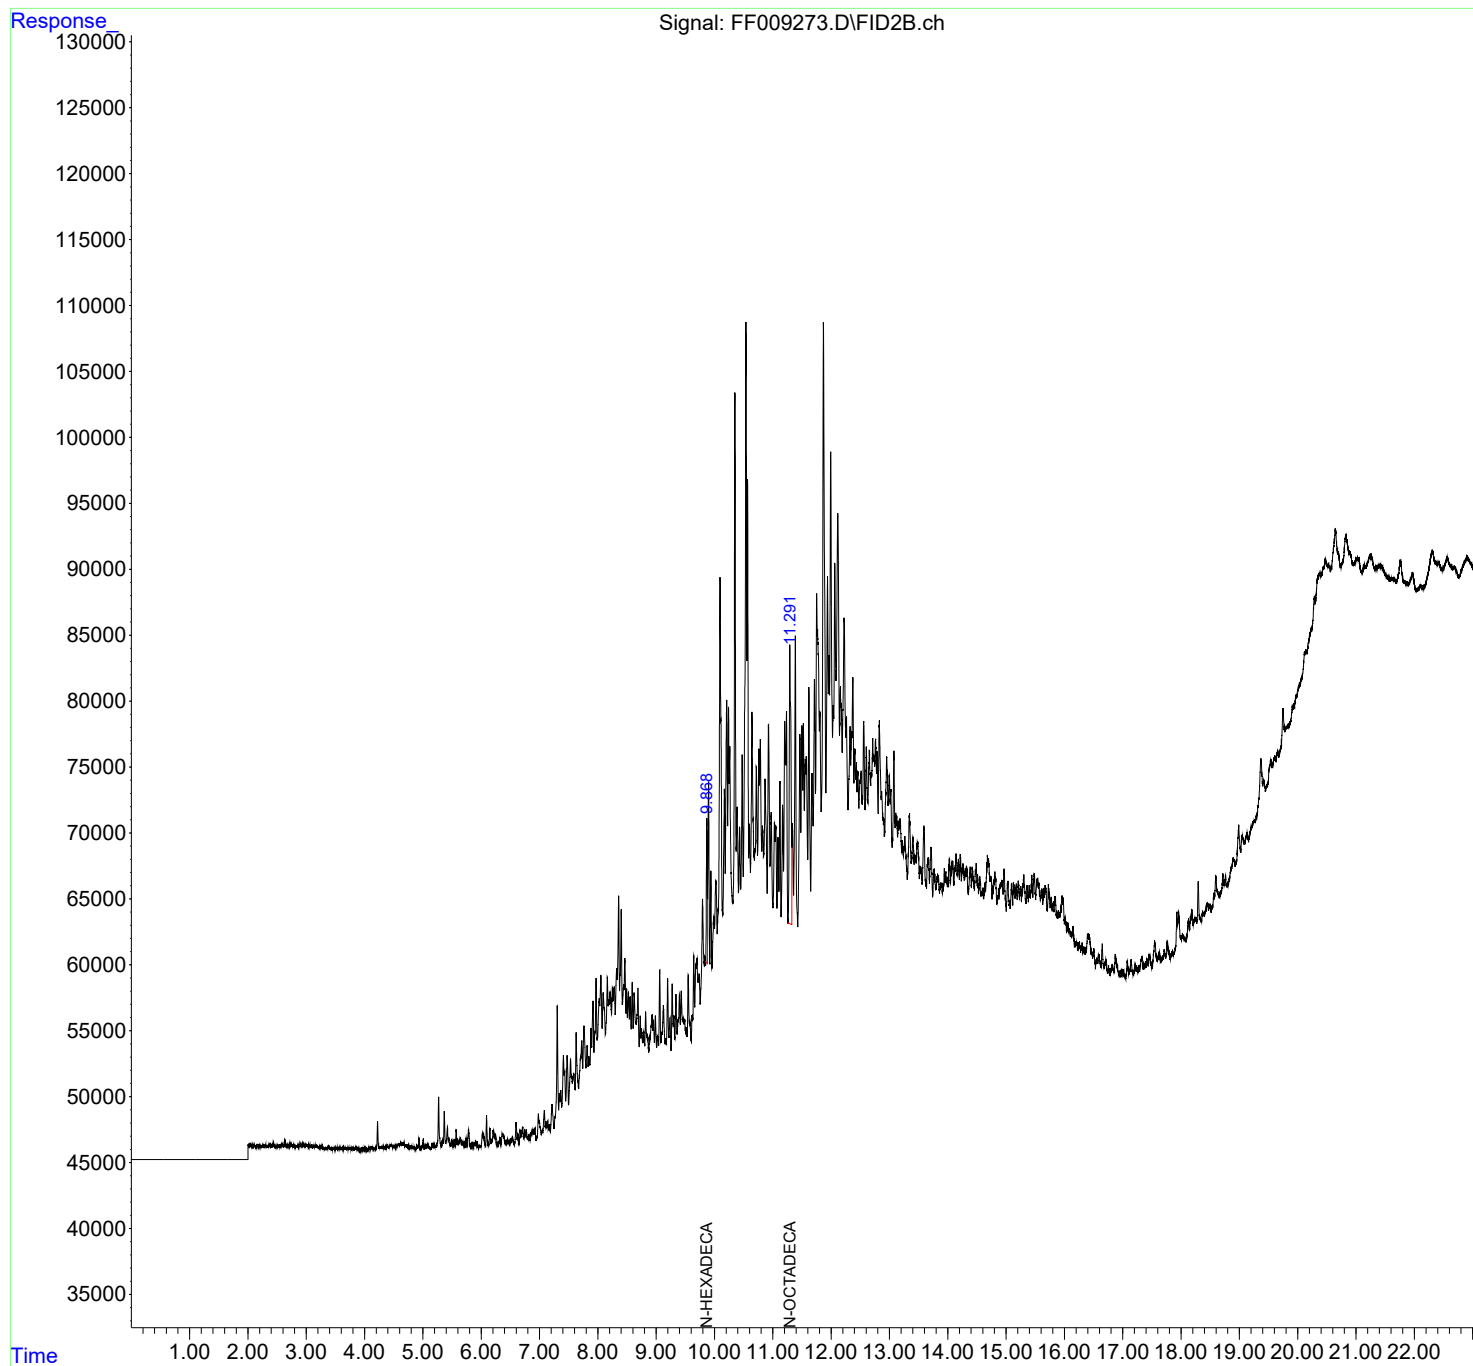


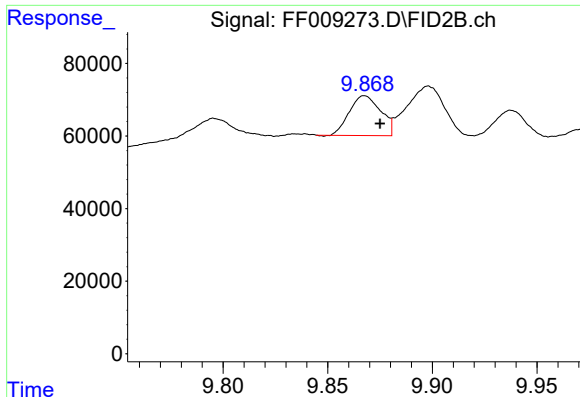

#5 N-HEXADECANE


R.T.: 9.868 min
Delta R.T.: -0.007 min
Response: 114122
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

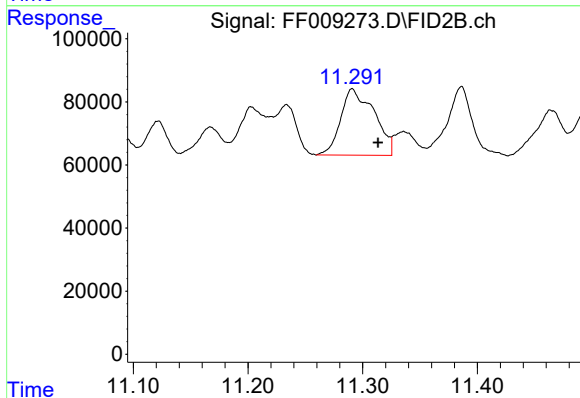

#6 N-OCTADECANE

R.T.: 11.291 min
Delta R.T.: -0.023 min
Response: 427077
Conc: 3.31 ug/ml

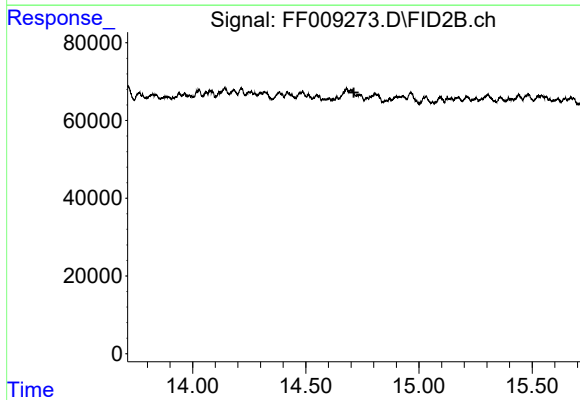

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.