

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110421\
Data File : FF009282.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2021 11:33
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 02:10:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.477	3510524	27.633 ug/ml
12)	N-OCTACOSANE	16.876	3603789	30.785 ug/ml
13)	N-TRIACONTANE	17.760	266963	2.366 ug/ml
14)	N-DOTRIACONTANE	18.590	350824	3.322 ug/ml
15)	N-TETRATRIACONTANE	19.370	303189	3.102 ug/ml
16)	N-HEXATRIACONTANE	20.111	199728	2.246 ug/ml
17)	N-OCTATRIACONTANE	20.845	130086	1.593 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110421\
Data File : FF009282.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2021 11:33
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 02:10:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

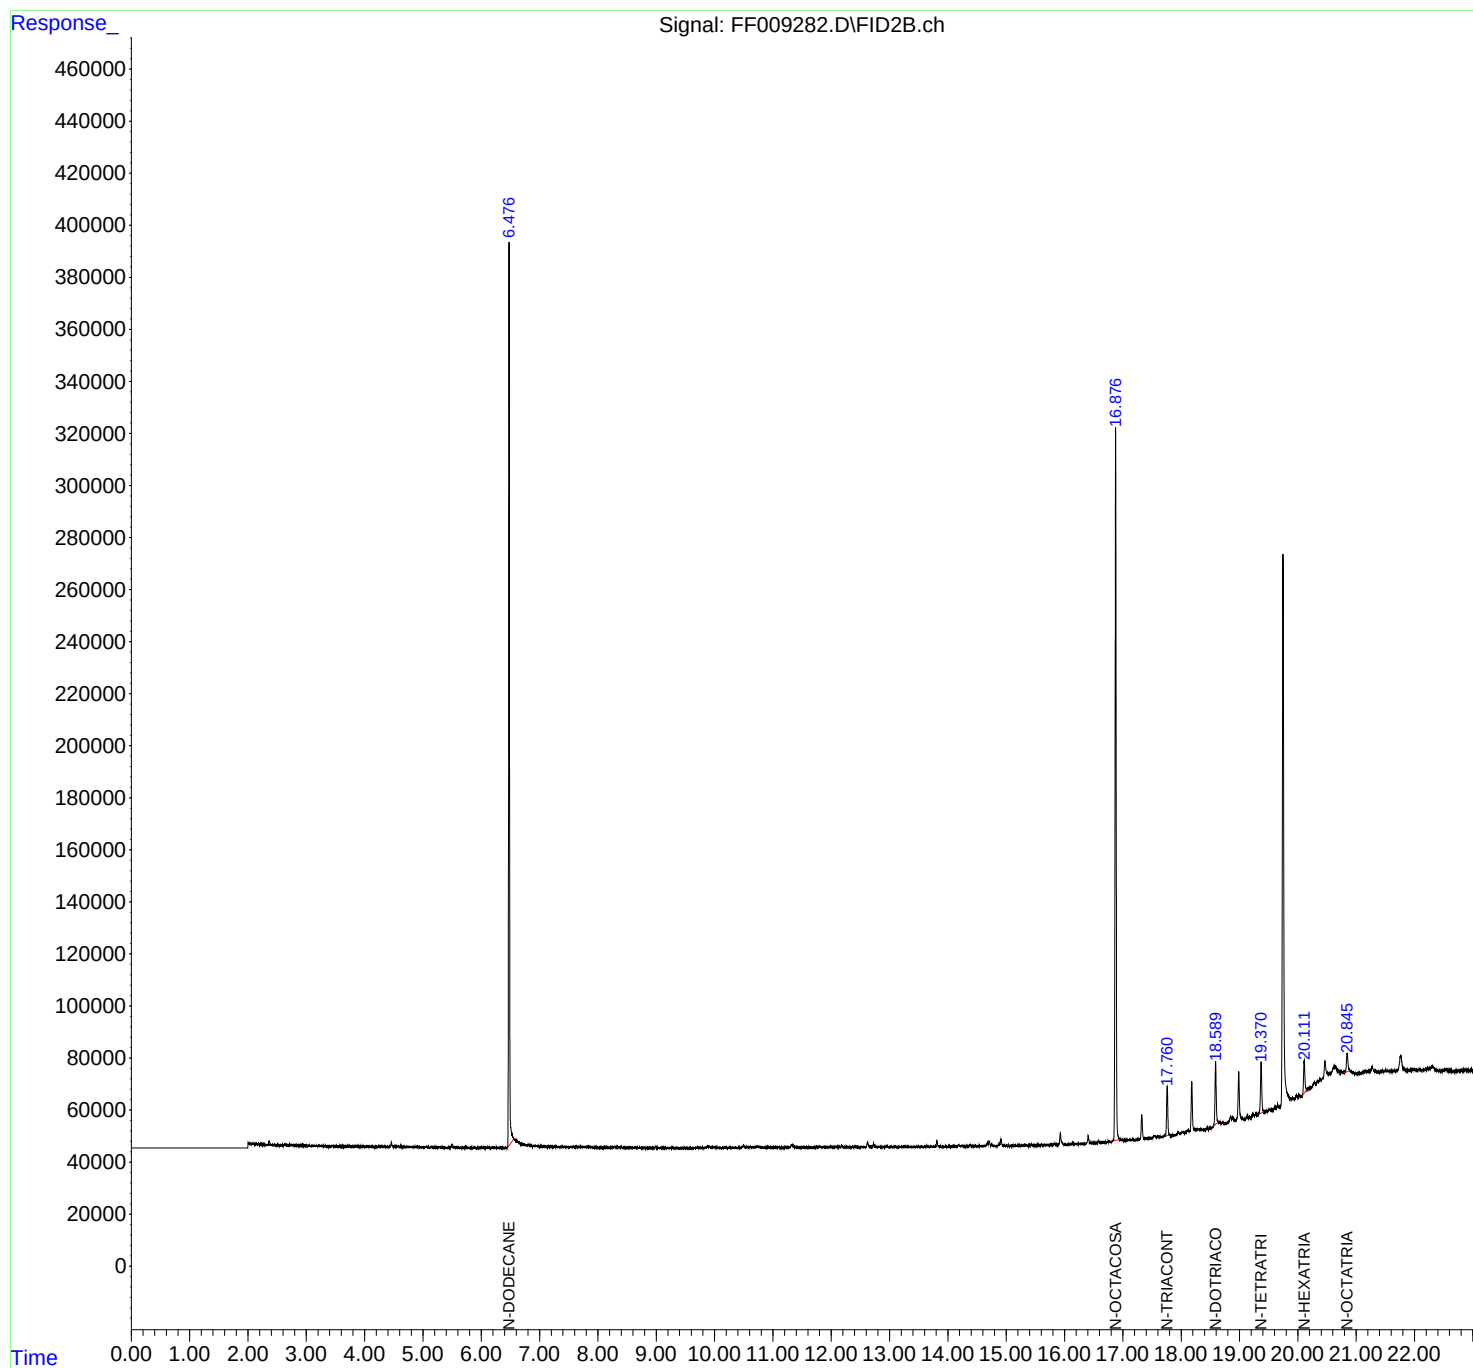


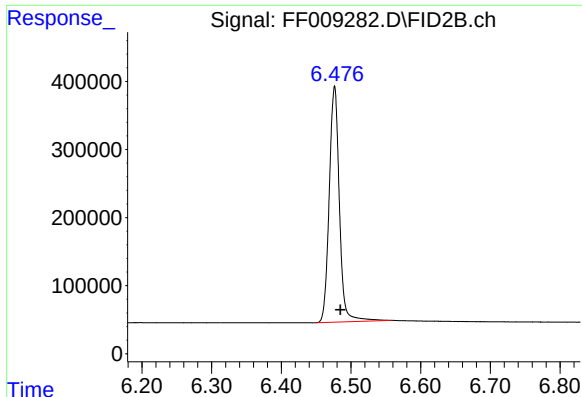

#3 N-DODECANE


R.T.: 6.477 min
Delta R.T.: -0.008 min
Response: 3510524
Conc: 27.63 ug/ml

Instrument :
FID_F
ClientSampleId :

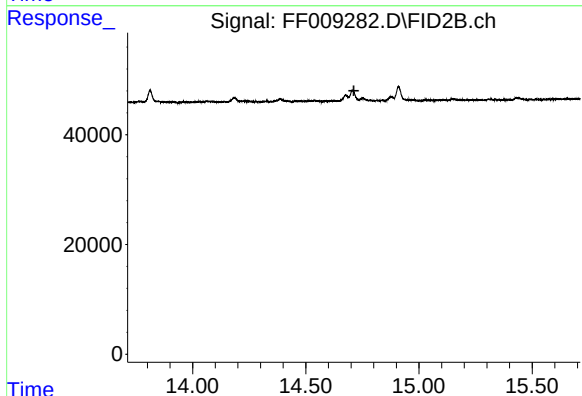


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

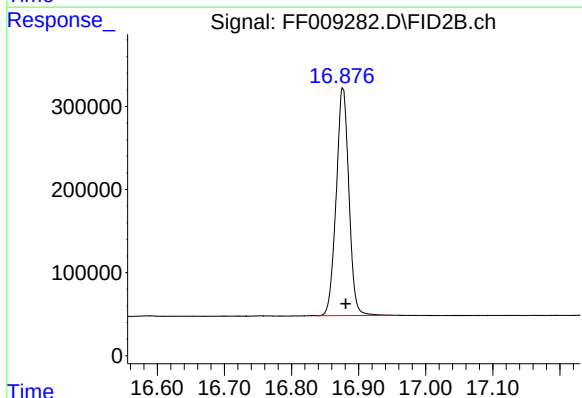


#12 N-OCTACOSANE

R.T.: 16.876 min
Delta R.T.: -0.005 min
Response: 3603789
Conc: 30.78 ug/ml

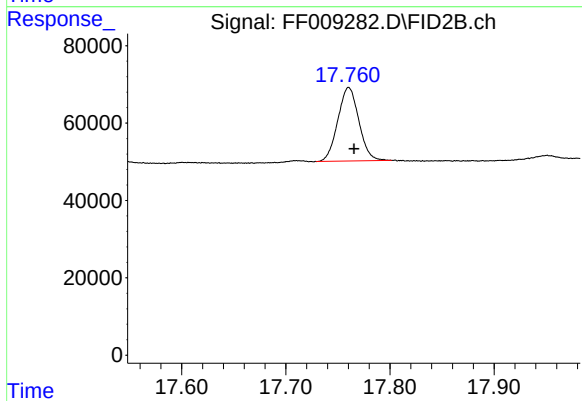

#13 N-TRIACONTANE


R.T.: 17.760 min
Delta R.T.: -0.005 min
Response: 266963
Conc: 2.37 ug/ml

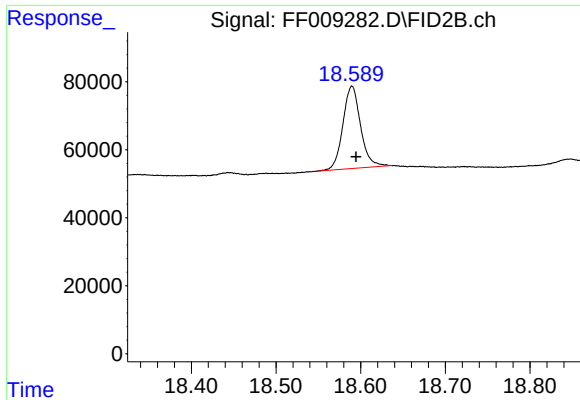

#14 N-DOTRIACONTANE


R.T.: 18.590 min
Delta R.T.: -0.005 min
Response: 350824
Conc: 3.32 ug/ml

Instrument :
FID_F
ClientSampleId :

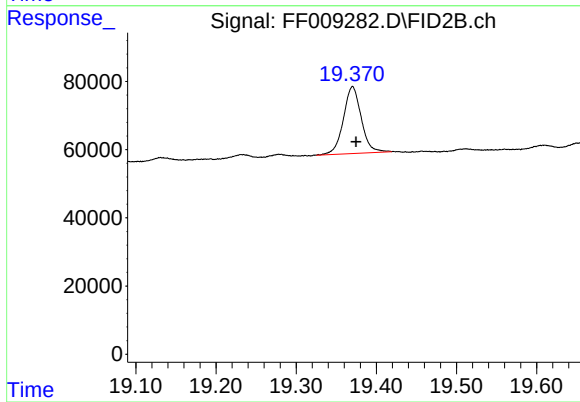


#15 N-TETRATRIACONTANE

R.T.: 19.370 min
Delta R.T.: -0.004 min
Response: 303189
Conc: 3.10 ug/ml

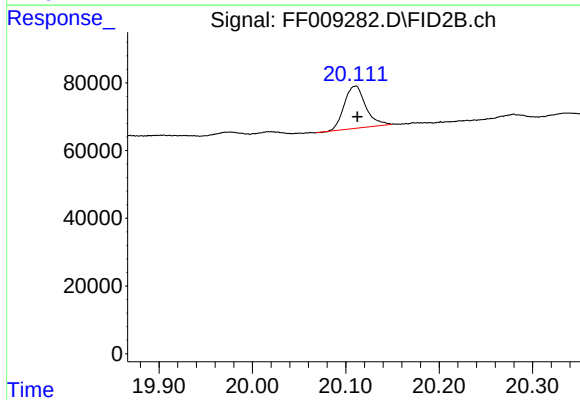

#16 N-HEXATRIACONTANE

R.T.: 20.111 min
Delta R.T.: -0.001 min
Response: 199728
Conc: 2.25 ug/ml

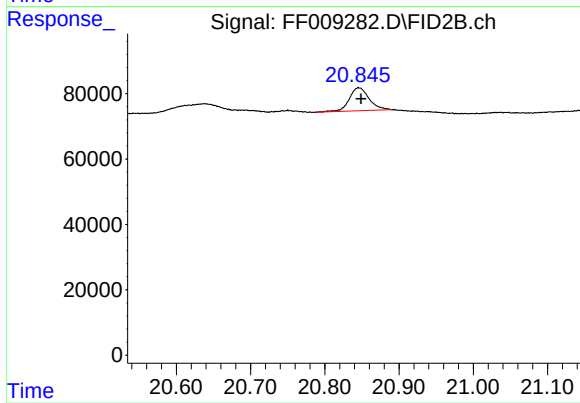

#17 N-OCTATRIACONTANE

R.T.: 20.845 min
Delta R.T.: -0.004 min
Response: 130086
Conc: 1.59 ug/ml