

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110421\
Data File : FF009289.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2021 15:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 02:12:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.707	1893006	17.263 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.762	118894	1.054 ug/ml
14)	N-DOTRIACONTANE	18.592	155290	1.471 ug/ml
15)	N-TETRATRIACONTANE	19.372	133598	1.367 ug/ml
16)	N-HEXATRIACONTANE	20.111	98517	1.108 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110421\
Data File : FF009289.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2021 15:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 02:12:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

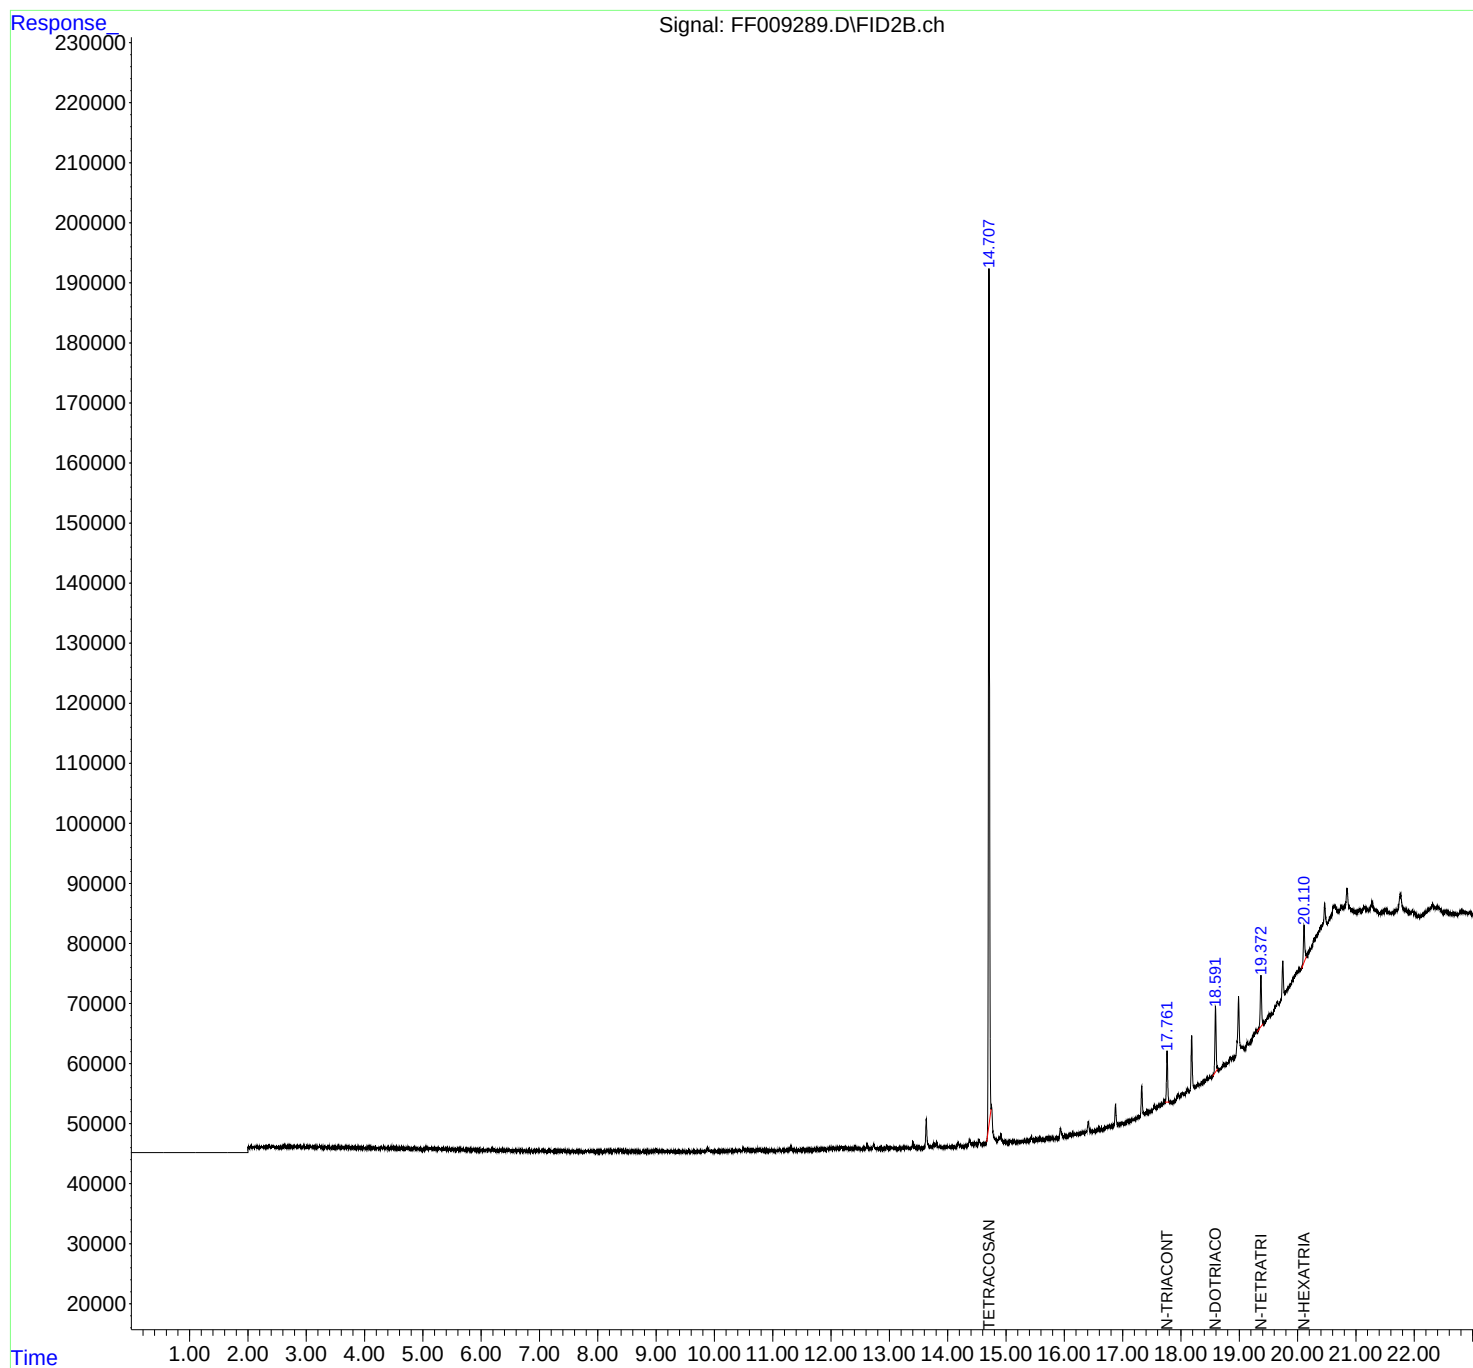


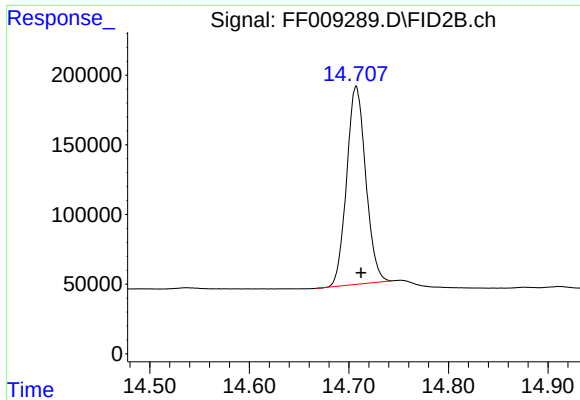

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.707 min
Delta R.T.: -0.005 min
Response: 1893006
Conc: 17.26 ug/ml

Instrument :
FID_F
ClientSampleId :

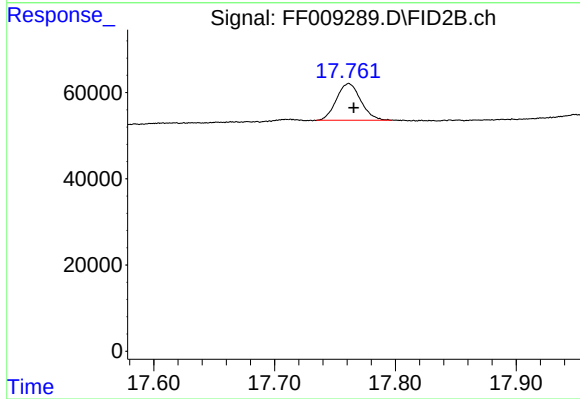


#13 N-TRIACONTANE

R.T.: 17.762 min
Delta R.T.: -0.004 min
Response: 118894
Conc: 1.05 ug/ml

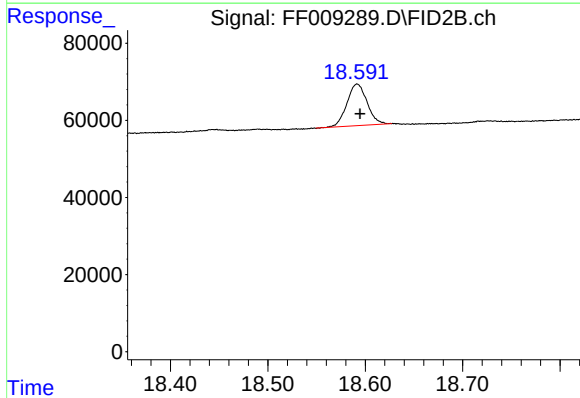


#14 N-DOTRIACONTANE

R.T.: 18.592 min
Delta R.T.: -0.003 min
Response: 155290
Conc: 1.47 ug/ml

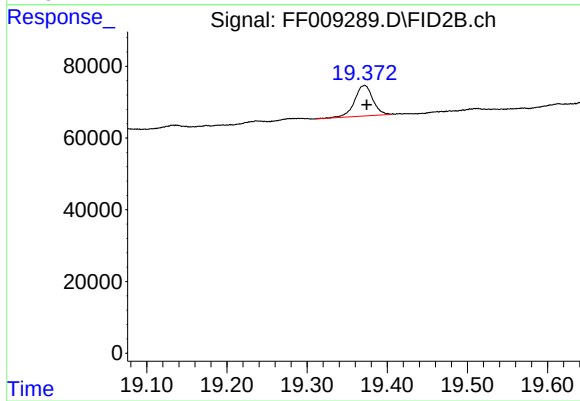

#15 N-TETRATRIACONTANE

R.T.: 19.372 min
Delta R.T.: -0.003 min
Response: 133598
Conc: 1.37 ug/ml

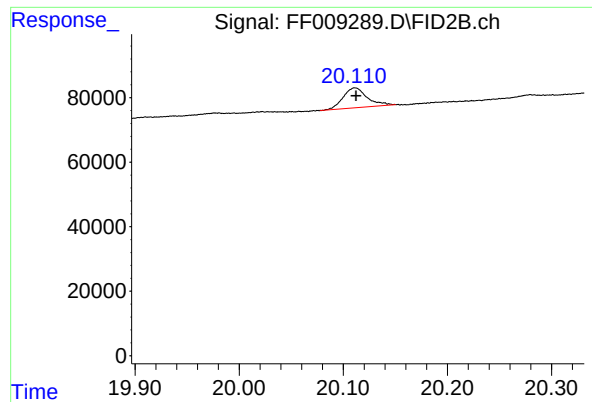

#16 N-HEXATRIACONTANE

R.T.: 20.111 min
Delta R.T.: -0.002 min
Response: 98517
Conc: 1.11 ug/ml

Instrument :

FID_F

ClientSampleId :