

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
Data File : FF011541.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2022 16:25
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 20:18:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.776	1712295	12.740 ug/ml
12)	N-OCTACOSANE	17.218	1826785	13.789 ug/ml
14)	N-DOTRIACONTANE	18.935	25654	0.191 ug/ml
15)	N-TETRATRIACONTANE	19.716	47909	0.364 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
Data File : FF011541.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2022 16:25
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 20:18:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

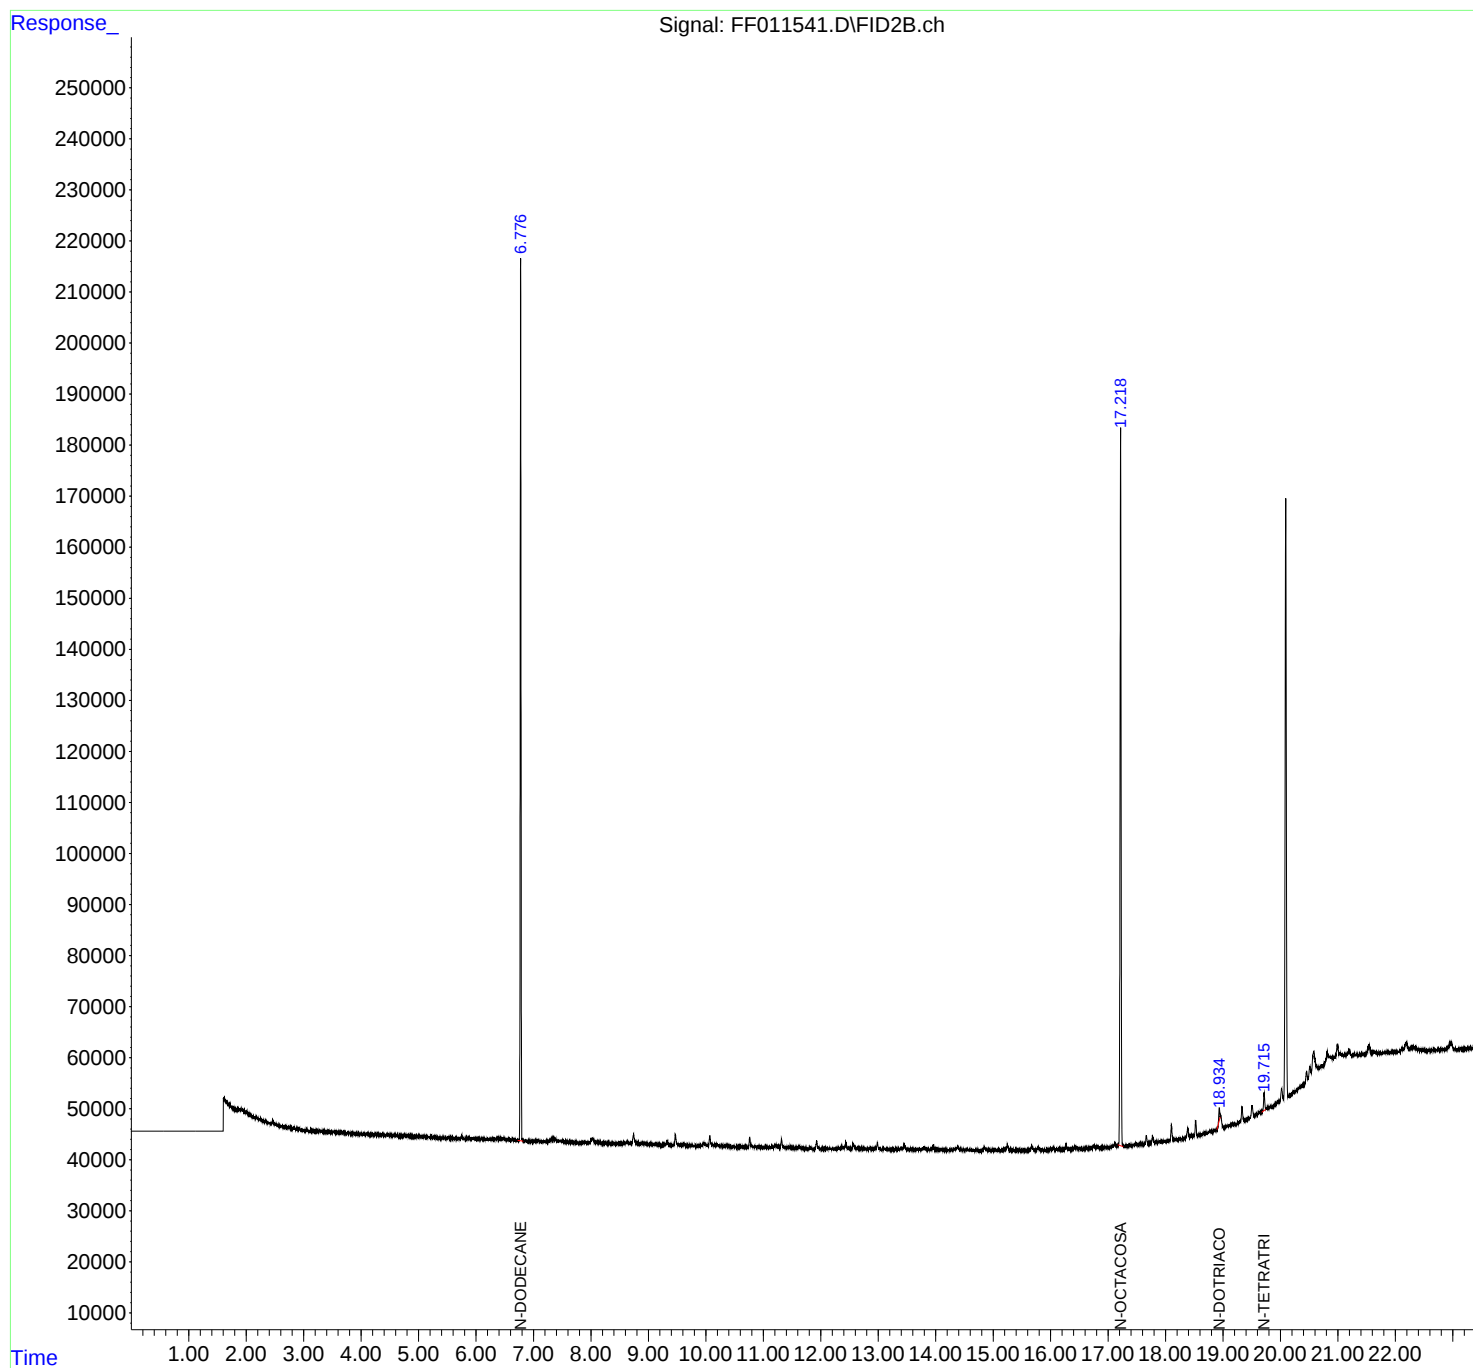


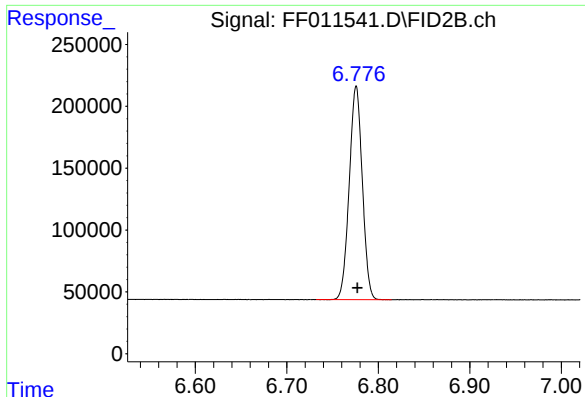

#3 N-DODECANE


R.T.: 6.776 min
Delta R.T.: -0.001 min
Response: 1712295
Conc: 12.74 ug/ml

Instrument :
FID_F
ClientSampleId :

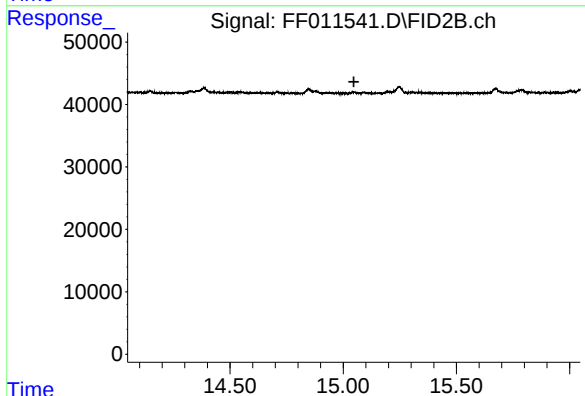


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

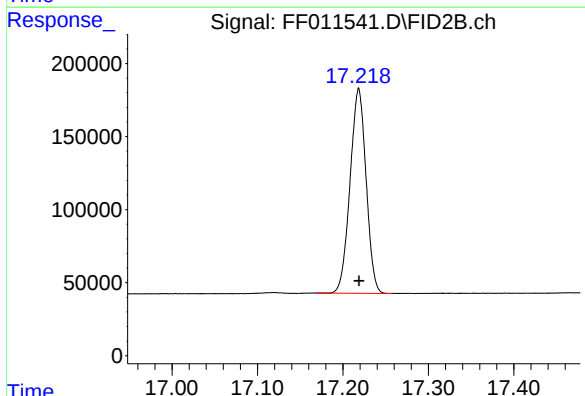


#12 N-OCTACOSANE

R.T.: 17.218 min
Delta R.T.: 0.000 min
Response: 1826785
Conc: 13.79 ug/ml

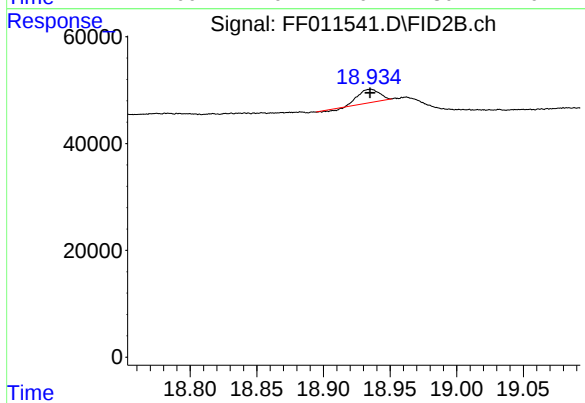

#14 N-DOTRIACONTANE

R.T.: 18.935 min
Delta R.T.: 0.000 min
Response: 25654
Conc: 0.19 ug/ml

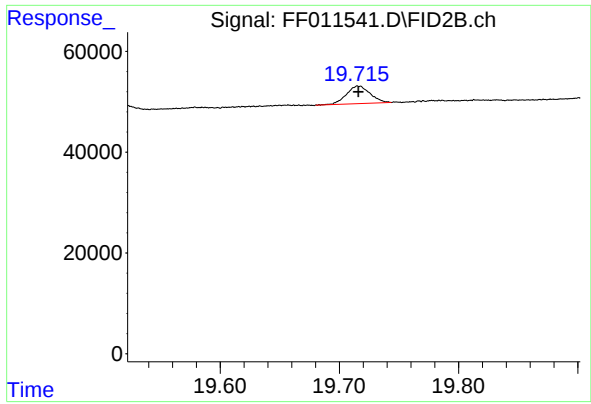

#15 N-TETRATRIACONTANE

R.T.: 19.716 min
Delta R.T.: 0.000 min
Response: 47909
Conc: 0.36 ug/ml

Instrument :

FID_F

ClientSampleId :