

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
 Data File : FF011544.D
 Signal(s) : FID2B.ch
 Acq On : 04 Nov 2022 17:54
 Operator : YP\AJ
 Sample : N5406-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 20:18:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.047	1429625	12.050 ug/ml
Target Compounds			
7) N-EICOSANE	13.011f	512474	3.706 ug/ml
8) N-DOCOSANE	14.147	26855	0.199 ug/ml
10) N-TETRACOSANE	15.248	120857	0.891 ug/ml
11) N-HEXACOSANE	16.269	177861	1.331 ug/ml
12) N-OCTACOSANE	17.217	201215	1.519 ug/ml
13) N-TRIACONTANE	18.104	162392	1.231 ug/ml
14) N-DOTRIACONTANE	18.935	177761	1.321 ug/ml
15) N-TETRATRIACONTANE	19.719	40004	0.304 ug/ml
16) N-HEXATRIACONTANE	20.457	49134	0.399 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
Data File : FF011544.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2022 17:54
Operator : YP\AJ
Sample : N5406-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 20:18:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

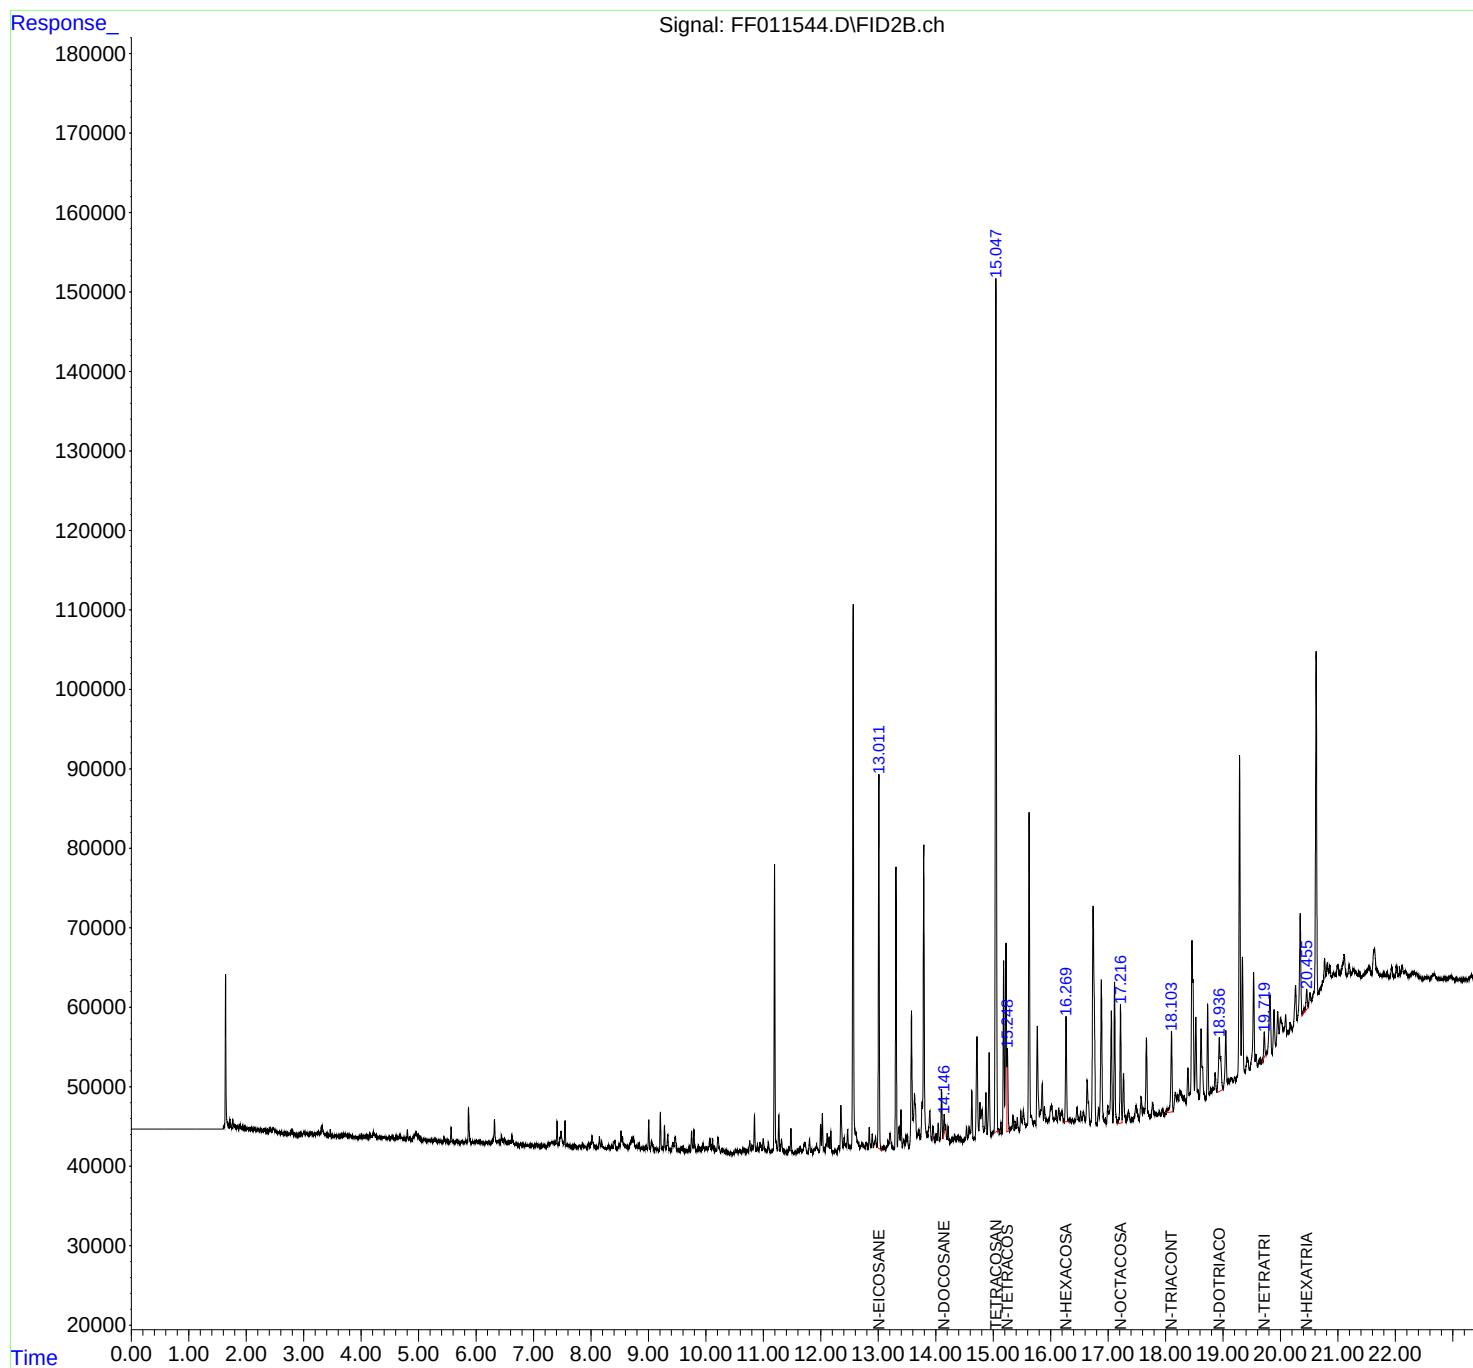


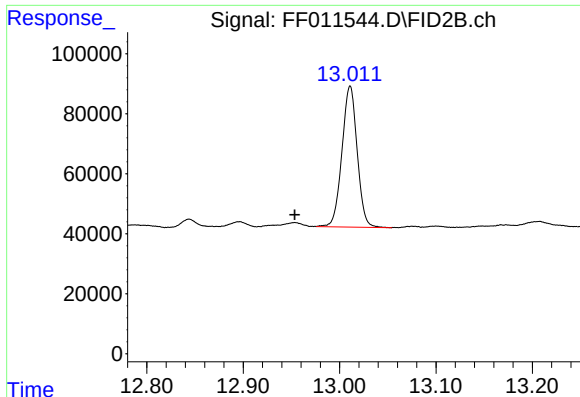

#7 N-EICOSANE


R.T.: 13.011 min
Delta R.T.: 0.058 min
Response: 512474
Conc: 3.71 ug/ml

Instrument :
FID_F
ClientSampleId :

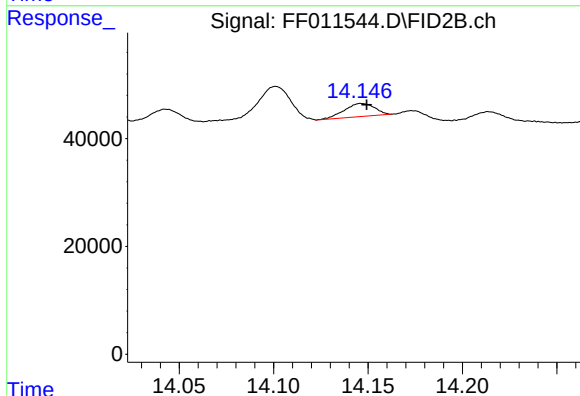


#8 N-DOCOSANE

R.T.: 14.147 min
Delta R.T.: -0.003 min
Response: 26855
Conc: 0.20 ug/ml

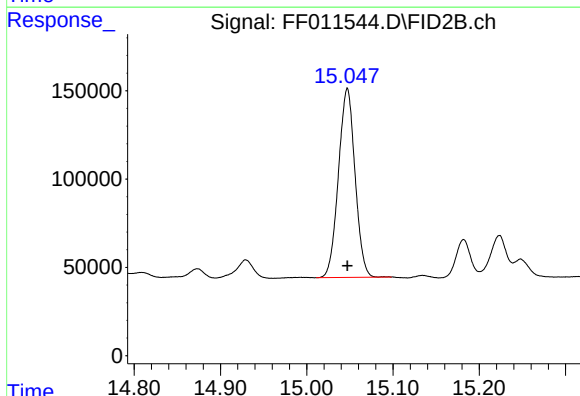


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.047 min
Delta R.T.: 0.000 min
Response: 1429625
Conc: 12.05 ug/ml

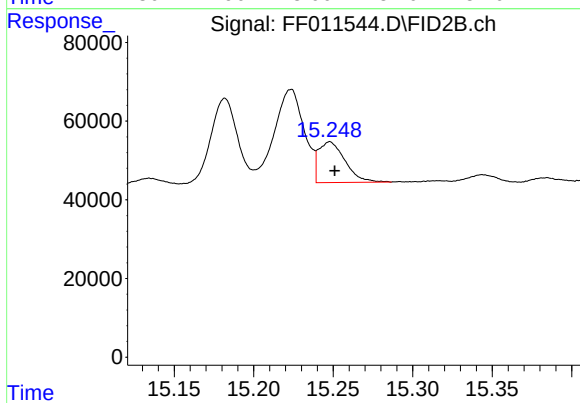

#10 N-TETRACOSANE


R.T.: 15.248 min
Delta R.T.: -0.003 min
Response: 120857
Conc: 0.89 ug/ml

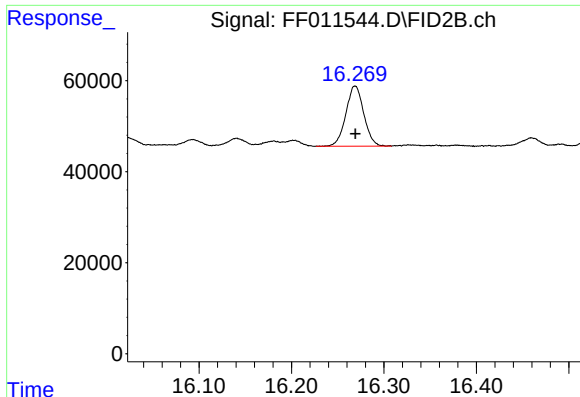

#11 N-HEXACOSANE


R.T.: 16.269 min
Delta R.T.: 0.000 min
Response: 177861
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :

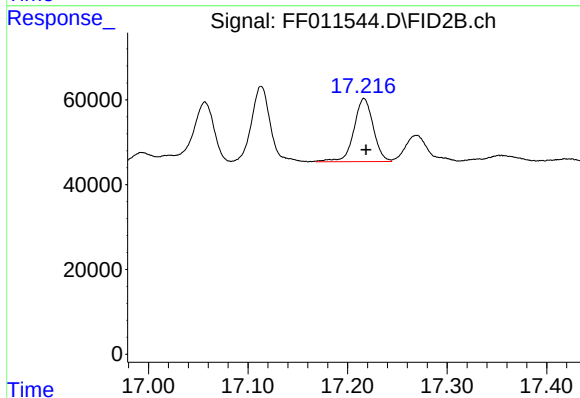


#12 N-OCTACOSANE

R.T.: 17.217 min
Delta R.T.: -0.002 min
Response: 201215
Conc: 1.52 ug/ml

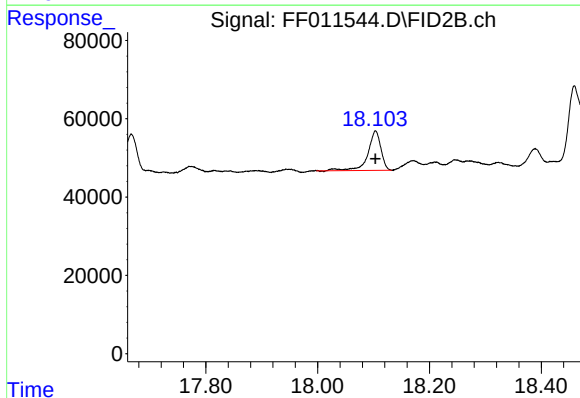


#13 N-TRIACONTANE

R.T.: 18.104 min
Delta R.T.: 0.000 min
Response: 162392
Conc: 1.23 ug/ml

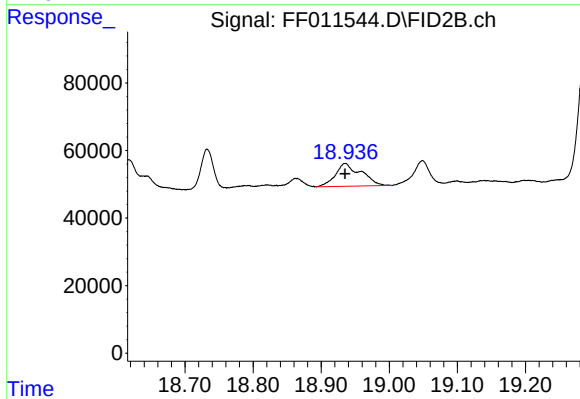

#14 N-DOTRIACONTANE


R.T.: 18.935 min
Delta R.T.: 0.000 min
Response: 177761
Conc: 1.32 ug/ml

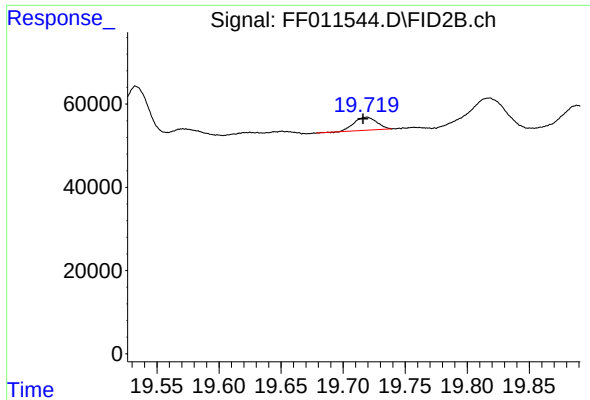

#15 N-TETRATRIACONTANE

R.T.: 19.719 min
Delta R.T.: 0.003 min
Response: 40004
Conc: 0.30 ug/ml

Instrument :
FID_F
ClientSampleId :

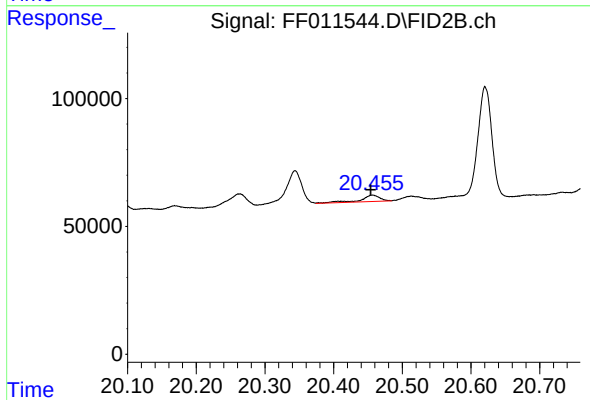

#16 N-HEXATRIACONTANE

R.T.: 20.457 min
Delta R.T.: 0.003 min
Response: 49134
Conc: 0.40 ug/ml