

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
 Data File : FF011545.D
 Signal(s) : FID2B.ch
 Acq On : 04 Nov 2022 18:24
 Operator : YP\AJ
 Sample : N5406-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 20:19:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.046	1851835	15.608 ug/ml
Target Compounds			
7) N-EICOSANE	13.010f	255372	1.847 ug/ml
8) N-DOCOSANE	14.147	27363	0.203 ug/ml
10) N-TETRACOSANE	15.248	127814	0.943 ug/ml
11) N-HEXACOSANE	16.268	176977	1.325 ug/ml
12) N-OCTACOSANE	17.216	206689	1.560 ug/ml
13) N-TRIACONTANE	18.104	228373	1.732 ug/ml
14) N-DOTRIACONTANE	18.935	260866	1.938 ug/ml
15) N-TETRATRIACONTANE	19.716	117839	0.895 ug/ml
16) N-HEXATRIACONTANE	20.456	78292	0.636 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
Data File : FF011545.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2022 18:24
Operator : YP\AJ
Sample : N5406-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 20:19:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

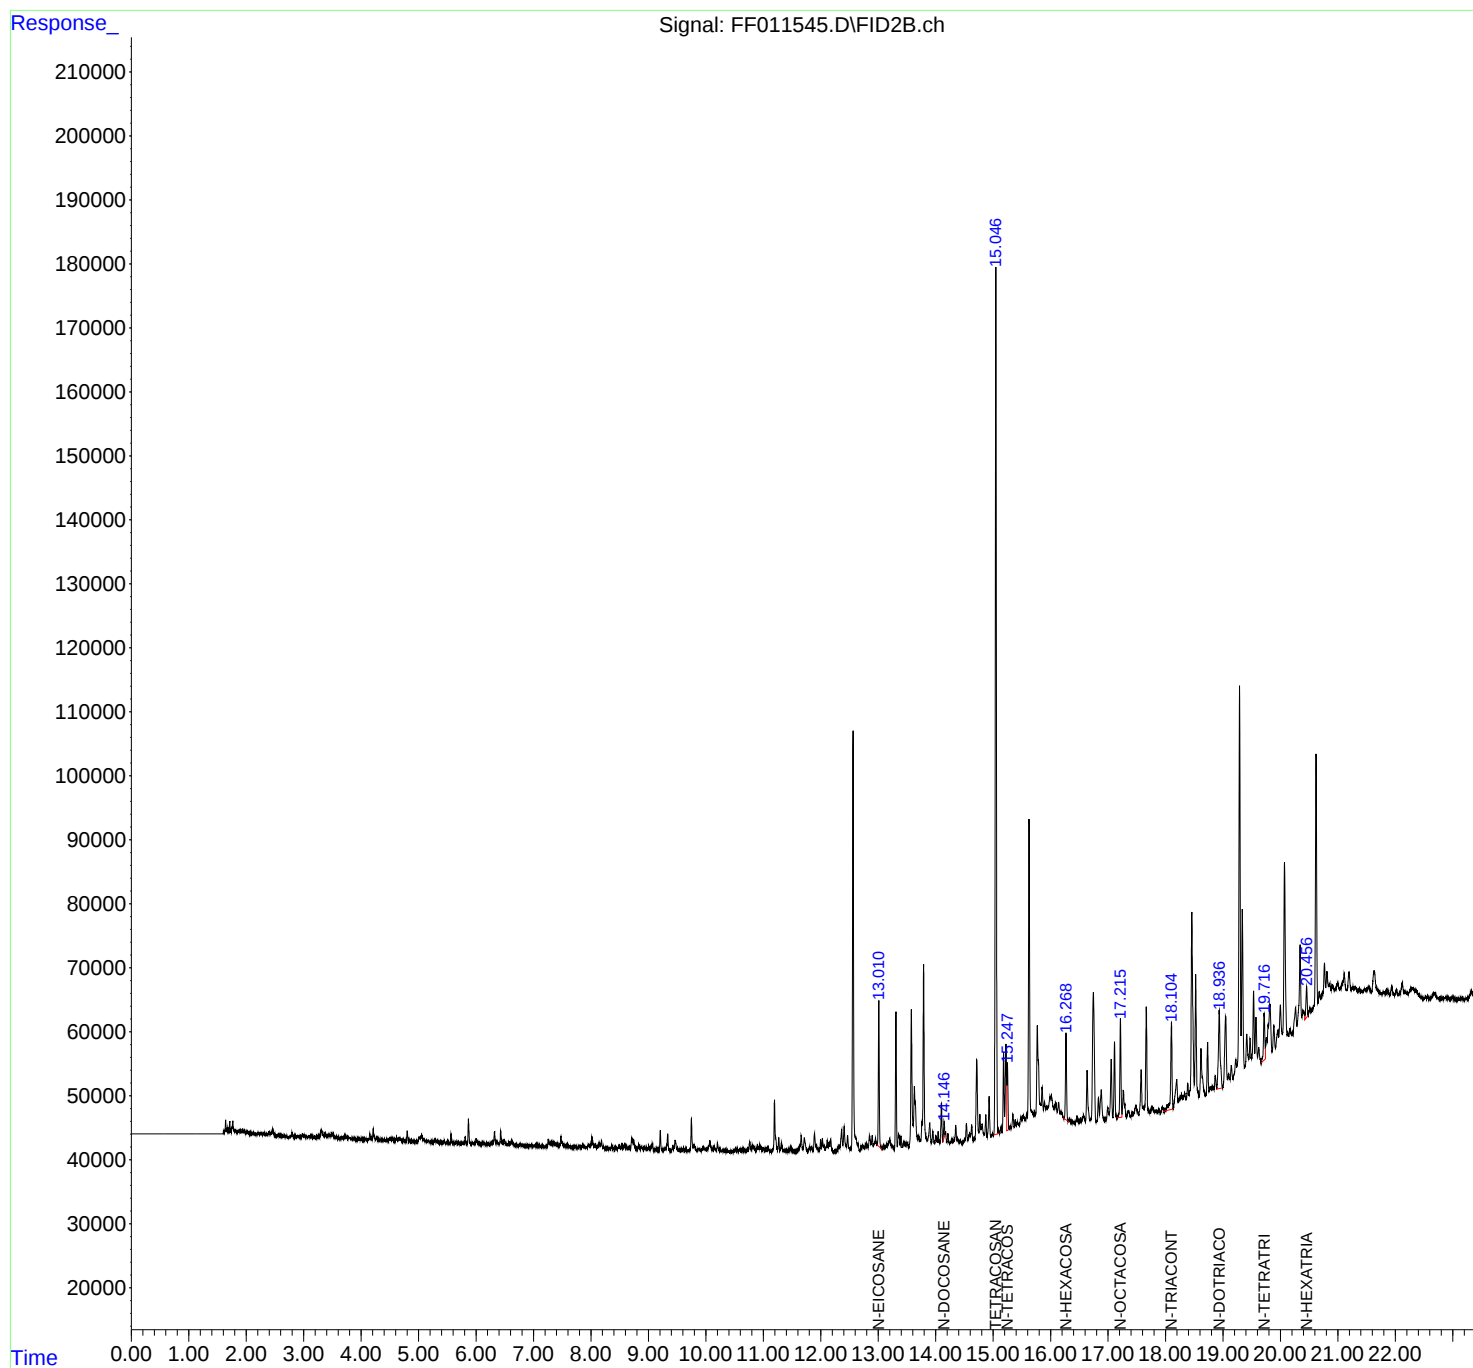


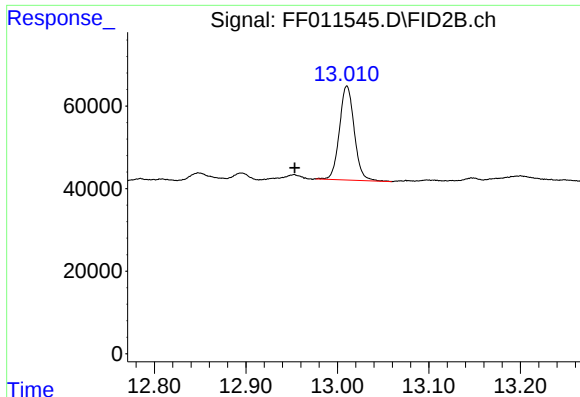

#7 N-EICOSANE


R.T.: 13.010 min
Delta R.T.: 0.057 min
Response: 255372
Conc: 1.85 ug/ml

Instrument :
FID_F
ClientSampleId :

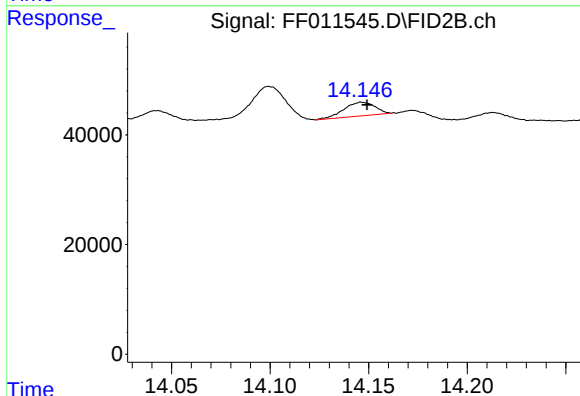


#8 N-DOCOSANE

R.T.: 14.147 min
Delta R.T.: -0.003 min
Response: 27363
Conc: 0.20 ug/ml

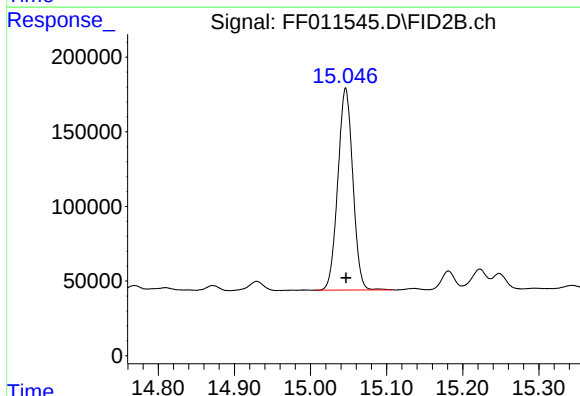


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: 0.000 min
Response: 1851835
Conc: 15.61 ug/ml

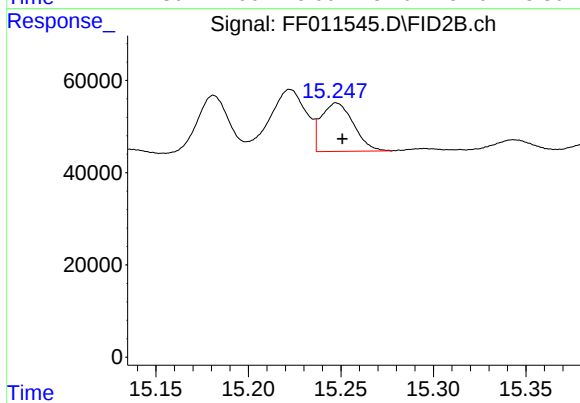

#10 N-TETRACOSANE


R.T.: 15.248 min
Delta R.T.: -0.003 min
Response: 127814
Conc: 0.94 ug/ml

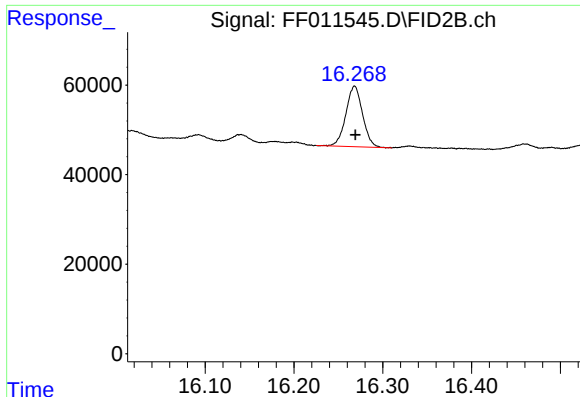

#11 N-HEXACOSANE


R.T.: 16.268 min
Delta R.T.: 0.000 min
Response: 176977
Conc: 1.32 ug/ml

Instrument :
FID_F
ClientSampleId :

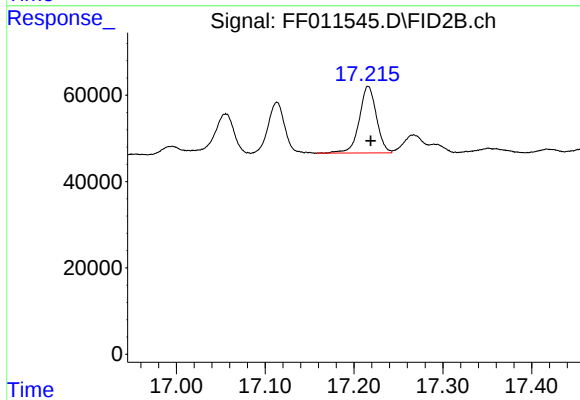


#12 N-OCTACOSANE

R.T.: 17.216 min
Delta R.T.: -0.003 min
Response: 206689
Conc: 1.56 ug/ml

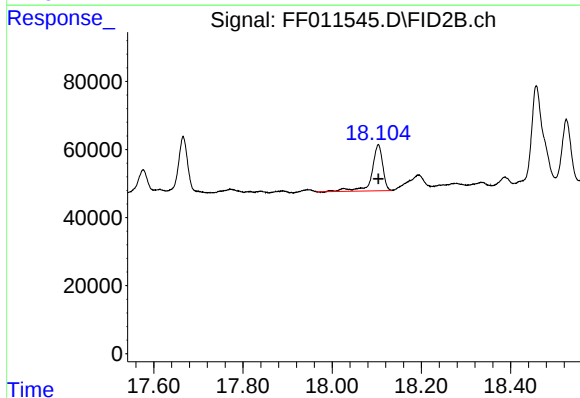


#13 N-TRIACONTANE

R.T.: 18.104 min
Delta R.T.: 0.000 min
Response: 228373
Conc: 1.73 ug/ml

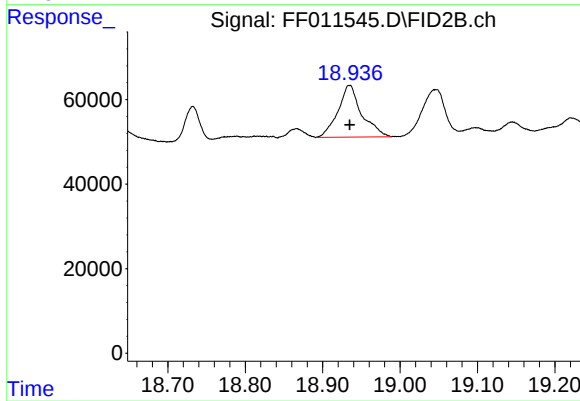

#14 N-DOTRIACONTANE


R.T.: 18.935 min
Delta R.T.: 0.000 min
Response: 260866
Conc: 1.94 ug/ml

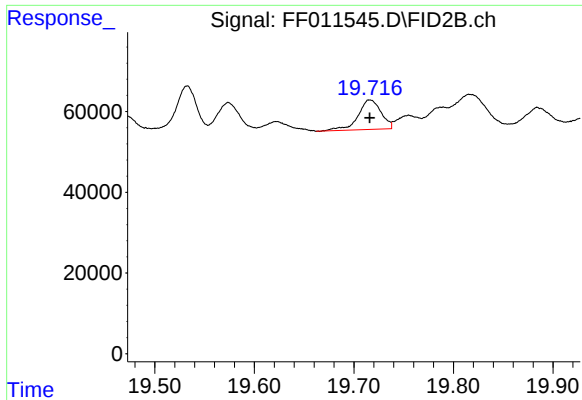

#15 N-TETRATRIACONTANE

R.T.: 19.716 min
Delta R.T.: 0.000 min
Response: 117839
Conc: 0.89 ug/ml

Instrument :
FID_F
ClientSampleId :

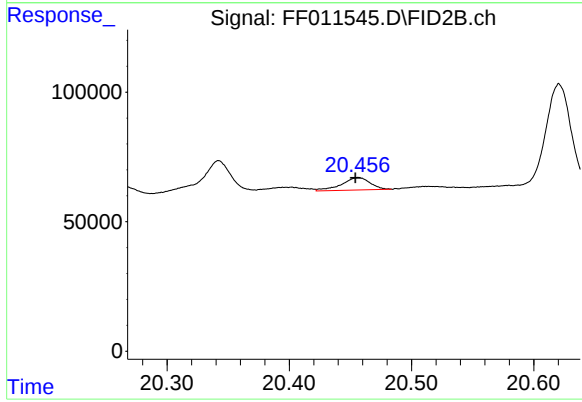

#16 N-HEXATRIACONTANE

R.T.: 20.456 min
Delta R.T.: 0.002 min
Response: 78292
Conc: 0.64 ug/ml