

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
 Data File : FF011548.D
 Signal(s) : FID2B.ch
 Acq On : 04 Nov 2022 19:53
 Operator : YP\AJ
 Sample : N5406-06
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 05 20:19:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.046	1310513	11.046 ug/ml
Target Compounds			
7) N-EICOSANE	13.010f	90806	0.657 ug/ml
8) N-DOCOSANE	14.099	55672	0.412 ug/ml
10) N-TETRACOSANE	15.248	93887	0.692 ug/ml
11) N-HEXACOSANE	16.268	125051	0.936 ug/ml
12) N-OCTACOSANE	17.215	137040	1.034 ug/ml
13) N-TRIACONTANE	18.102	132926	1.008 ug/ml
14) N-DOTRIACONTANE	18.925	290135	2.156 ug/ml
16) N-HEXATRIACONTANE	20.502	77339	0.628 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110422\
Data File : FF011548.D
Signal(s) : FID2B.ch
Acq On : 04 Nov 2022 19:53
Operator : YP\AJ
Sample : N5406-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 05 20:19:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

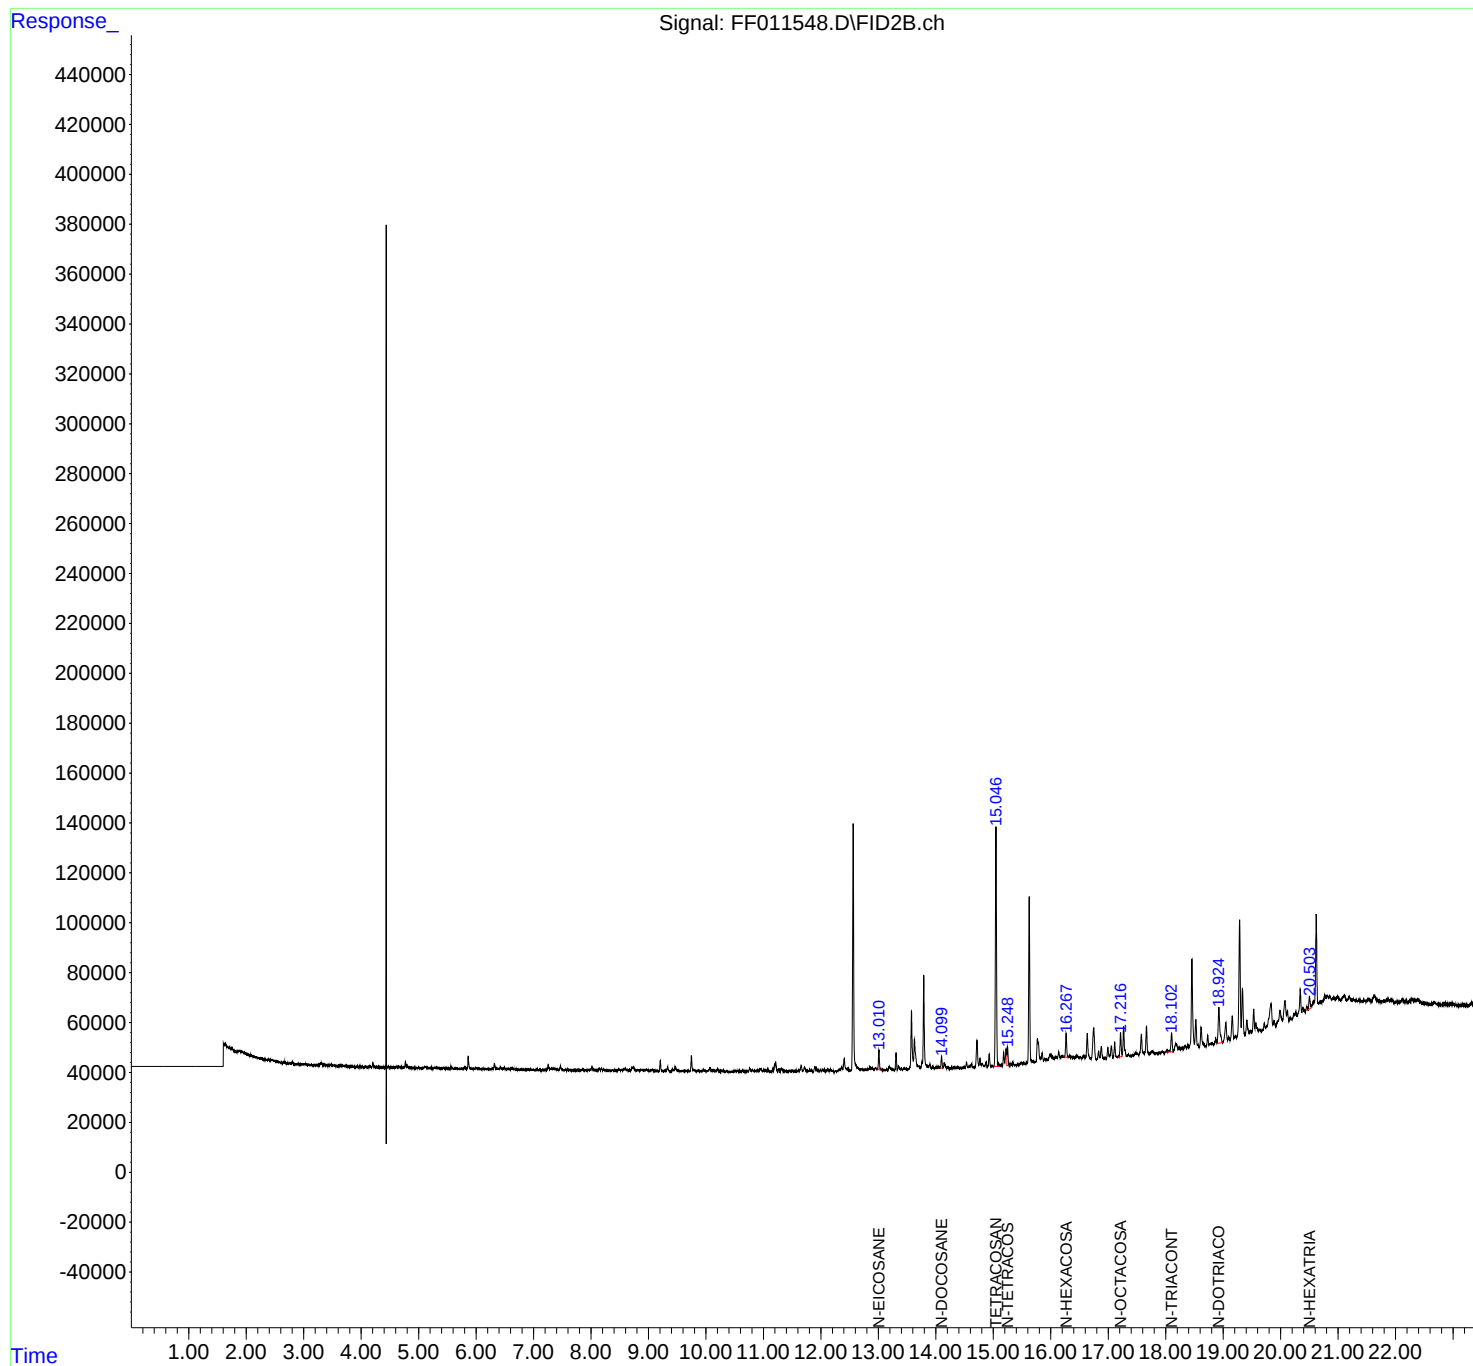


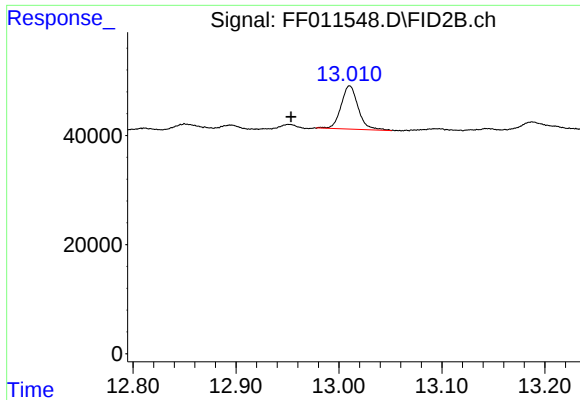

#7 N-EICOSANE


R.T.: 13.010 min
Delta R.T.: 0.057 min
Response: 90806
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

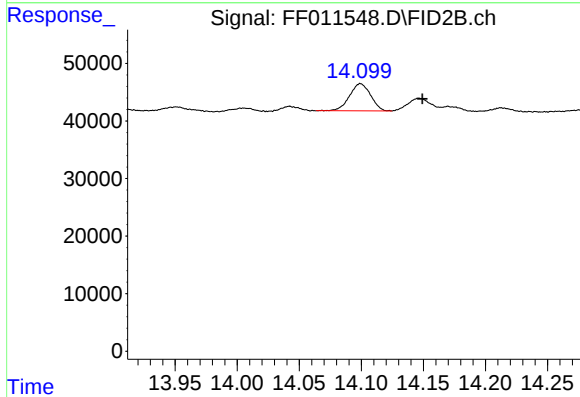


#8 N-DOCOSANE

R.T.: 14.099 min
Delta R.T.: -0.050 min
Response: 55672
Conc: 0.41 ug/ml

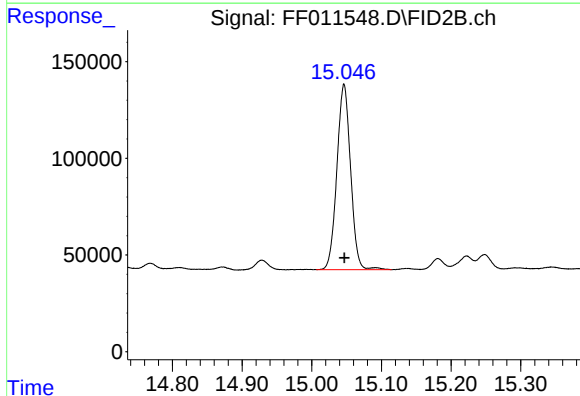


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: 0.000 min
Response: 1310513
Conc: 11.05 ug/ml

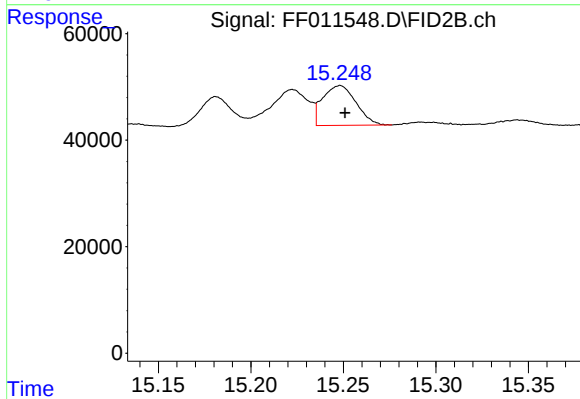

#10 N-TETRACOSANE


R.T.: 15.248 min
Delta R.T.: -0.003 min
Response: 93887
Conc: 0.69 ug/ml

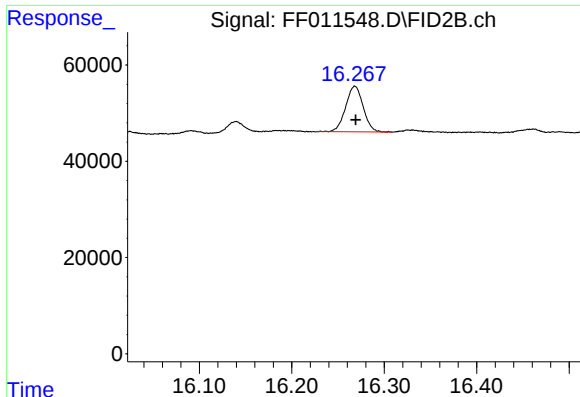

#11 N-HEXACOSANE


R.T.: 16.268 min
Delta R.T.: 0.000 min
Response: 125051
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

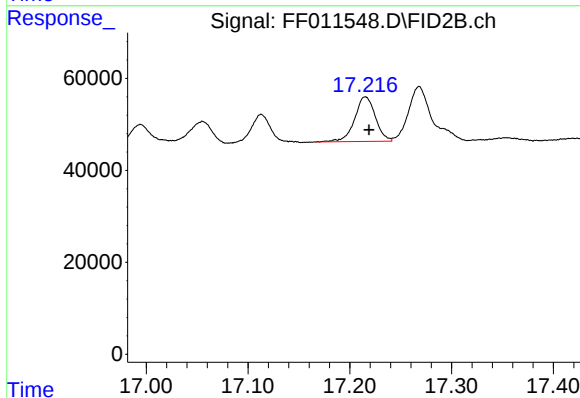


#12 N-OCTACOSANE

R.T.: 17.215 min
Delta R.T.: -0.003 min
Response: 137040
Conc: 1.03 ug/ml

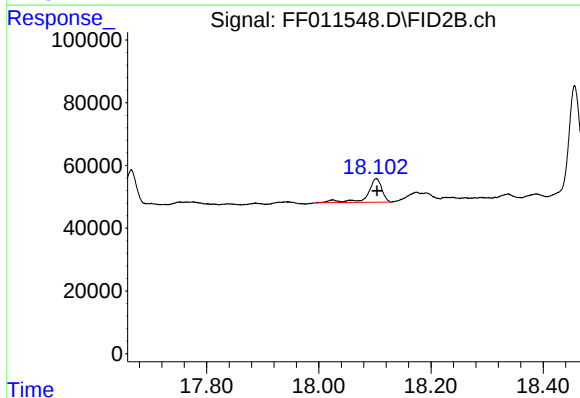


#13 N-TRIACONTANE

R.T.: 18.102 min
Delta R.T.: -0.001 min
Response: 132926
Conc: 1.01 ug/ml

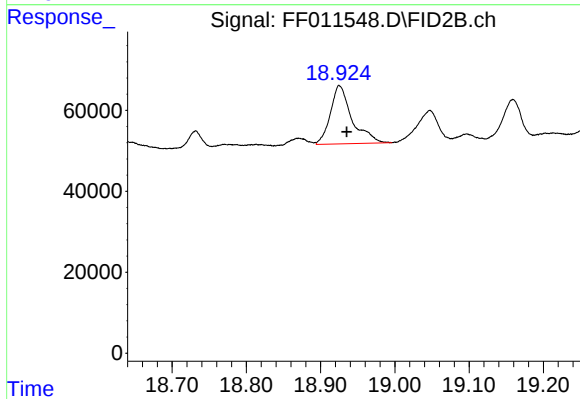

#14 N-DOTRIACONTANE

R.T.: 18.925 min
Delta R.T.: -0.010 min
Response: 290135
Conc: 2.16 ug/ml

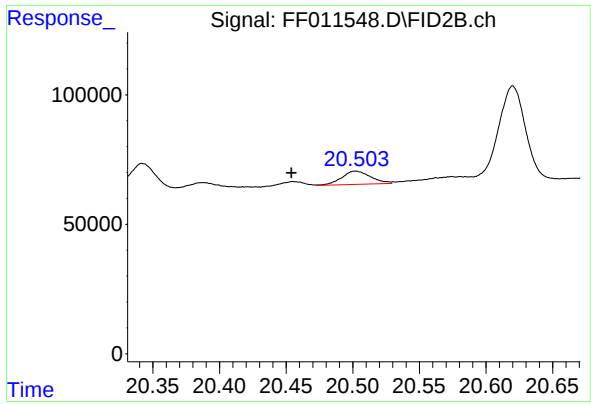

#16 N-HEXATRIACONTANE

R.T.: 20.502 min
Delta R.T.: 0.048 min
Response: 77339
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :