

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110618\
Data File : FF002598.D
Signal(s) : FID2B.ch
Acq On : 07 Nov 2018 02:50
Operator : AJ\SJ
Sample : J5827-43
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 09:46:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.627	2593177	20.661 ug/ml
Target Compounds				
6)	N-TETRADECANE	8.240	1115580	10.071 ug/ml
9)	N-EICOSANE	12.580	200377	1.796 ug/ml
11)	N-OCTACOSANE	16.799	608839	5.830 ug/ml
12)	N-DOTRIACONTANE	18.518	455768	4.793 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110618\
Data File : FF002598.D
Signal(s) : FID2B.ch
Acq On : 07 Nov 2018 02:50
Operator : AJ\SJ
Sample : J5827-43
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 09:46:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

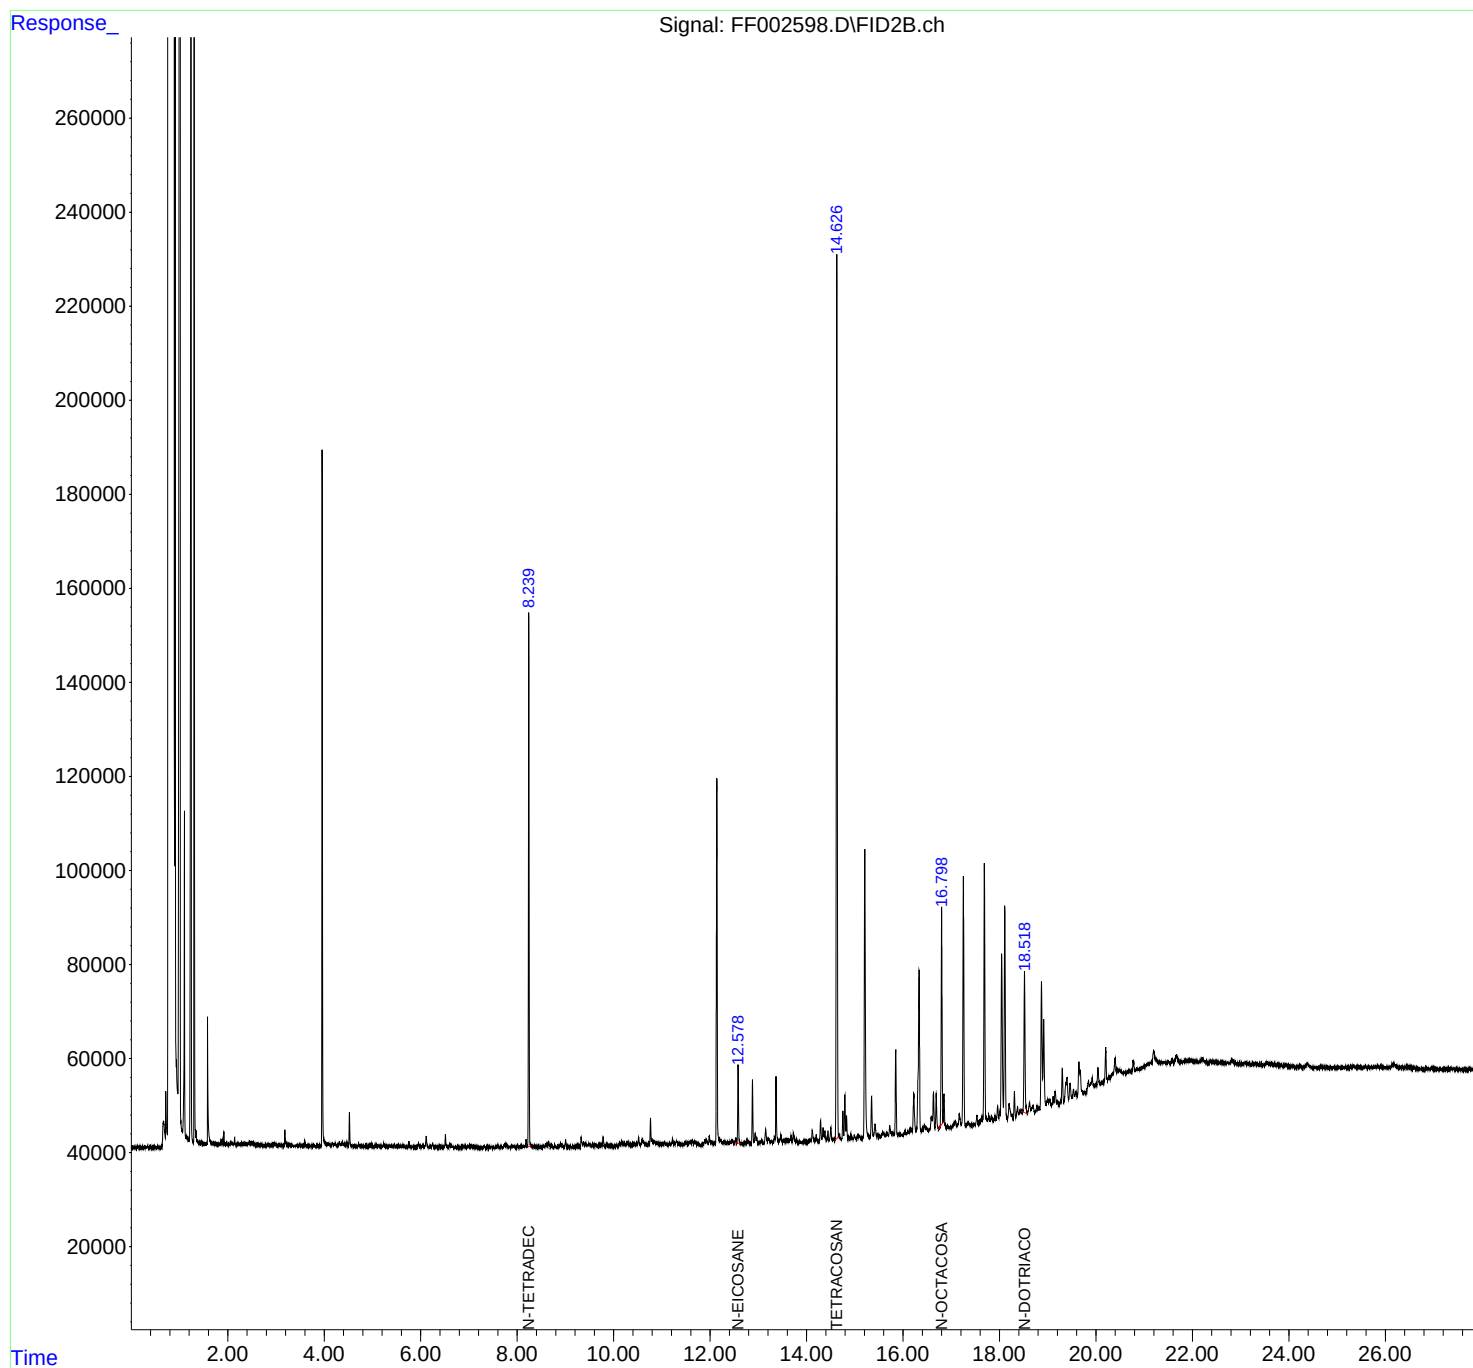

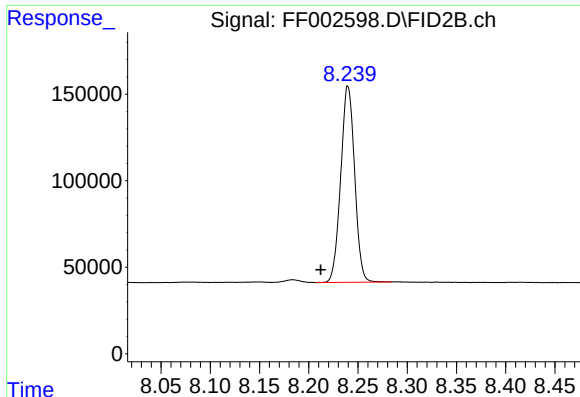


#6 N-TETRADECANE

R.T.: 8.240 min
Delta R.T.: 0.028 min
Response: 1115580
Conc: 10.07 ug/ml

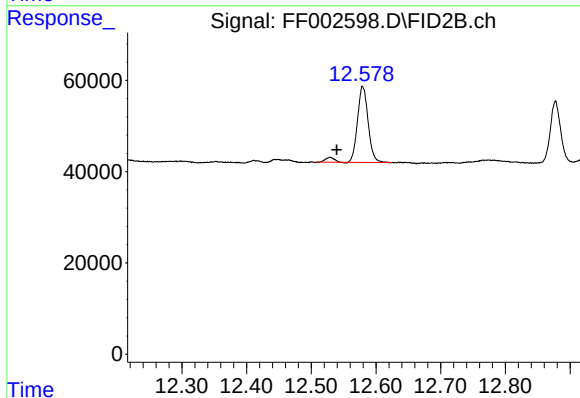


#9 N-EICOSANE

R.T.: 12.580 min
Delta R.T.: 0.040 min
Response: 200377
Conc: 1.80 ug/ml

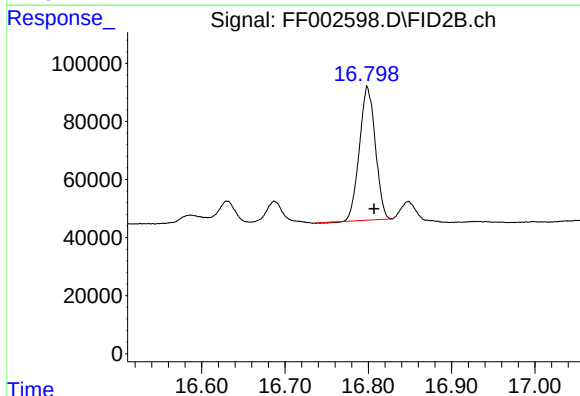


#11 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: -0.008 min
Response: 608839
Conc: 5.83 ug/ml

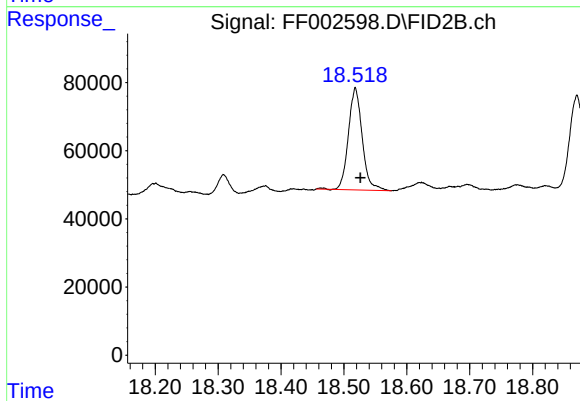

#12 N-DOTRIACONTANE

R.T.: 18.518 min
Delta R.T.: -0.008 min
Response: 455768
Conc: 4.79 ug/ml

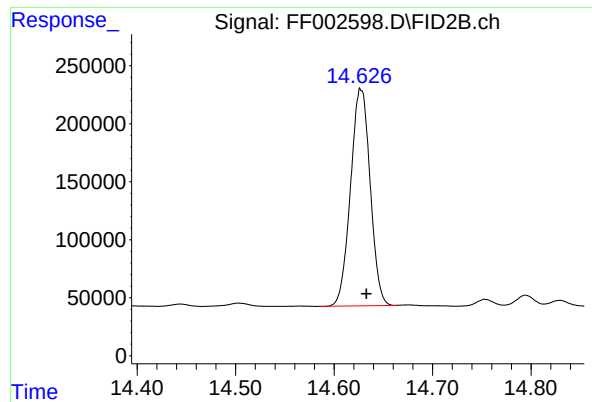

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.006 min
Response: 2593177
Conc: 20.66 ug/ml