

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110618\
Data File : FF002605.D
Signal(s) : FID2B.ch
Acq On : 07 Nov 2018 06:55
Operator : AJ\SJ
Sample : J5827-42
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 09:46:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.624	2571279	20.486 ug/ml
Target Compounds				
6)	N-TETRADECANE	8.238	1089512	9.835 ug/ml
9)	N-EICOSANE	12.576	190796	1.711 ug/ml
11)	N-OCTACOSANE	16.794	608122	5.823 ug/ml
12)	N-DOTRIACONTANE	18.513	453988	4.774 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110618\
Data File : FF002605.D
Signal(s) : FID2B.ch
Acq On : 07 Nov 2018 06:55
Operator : AJ\SJ
Sample : J5827-42
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 09:46:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

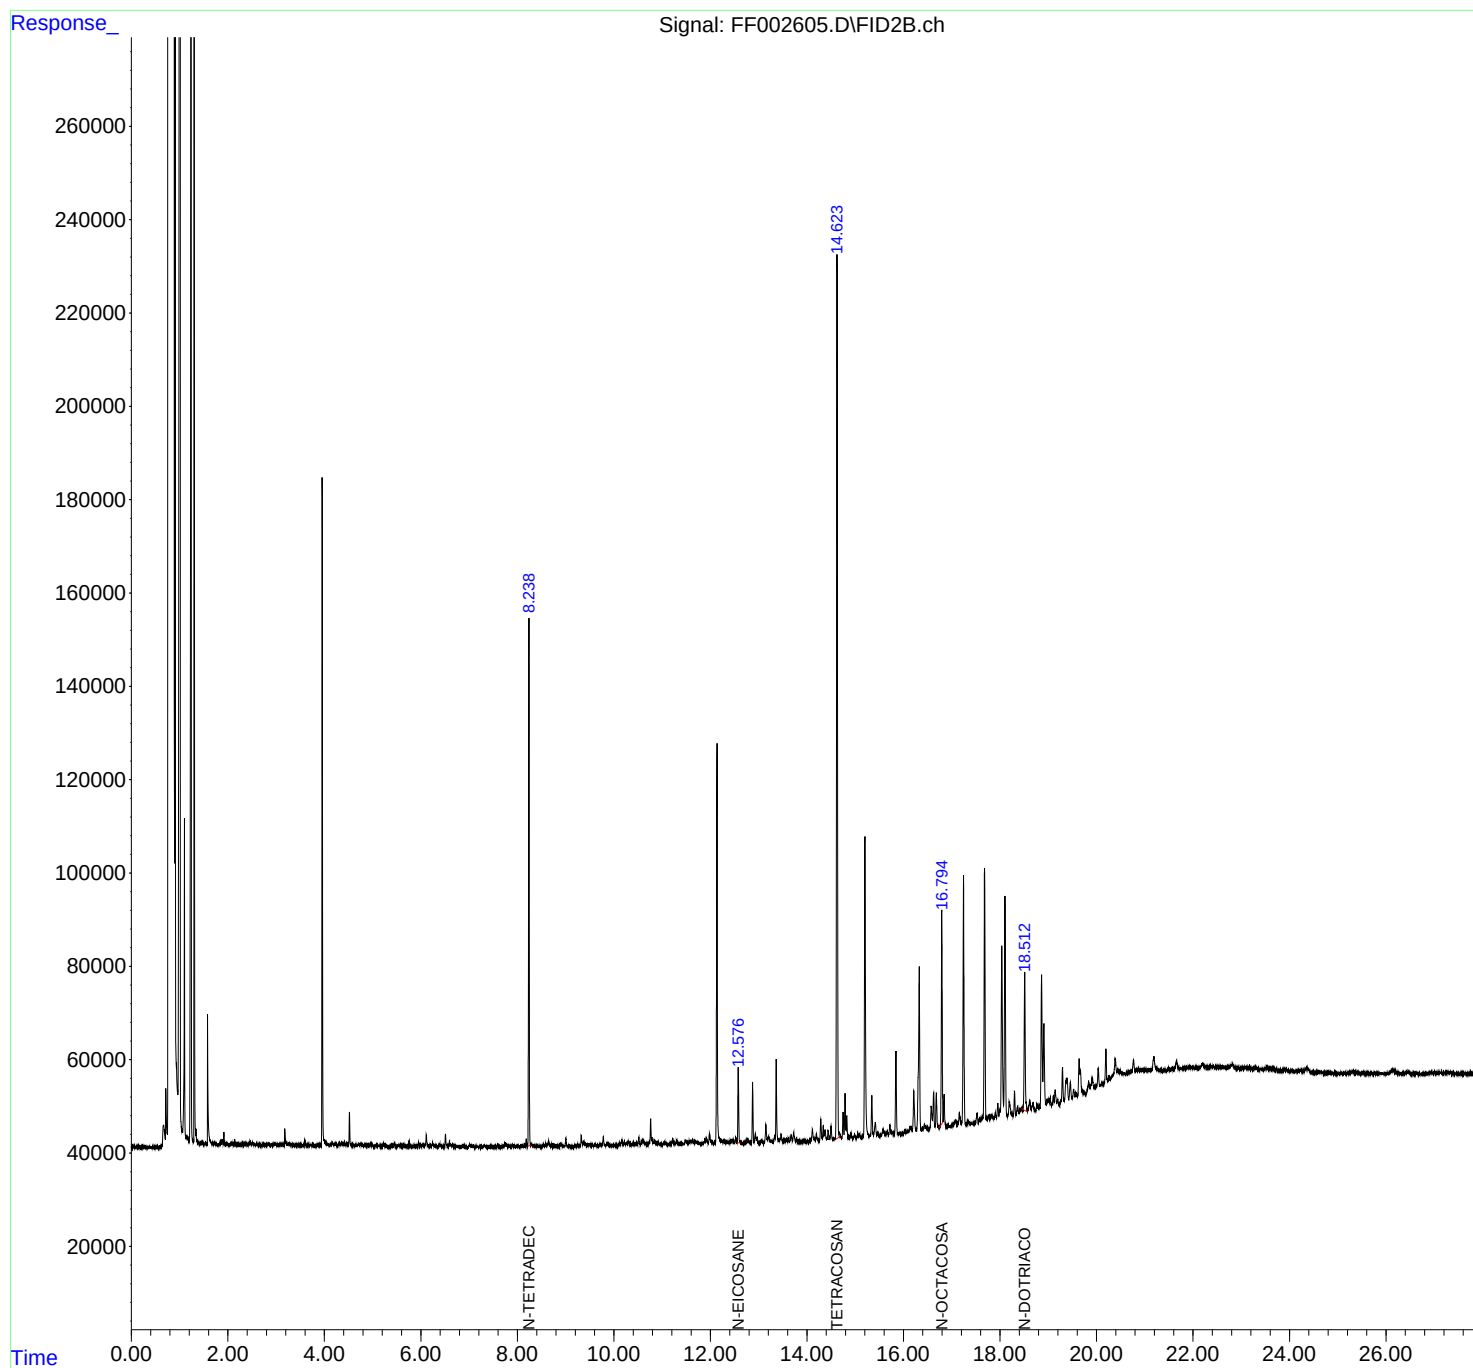

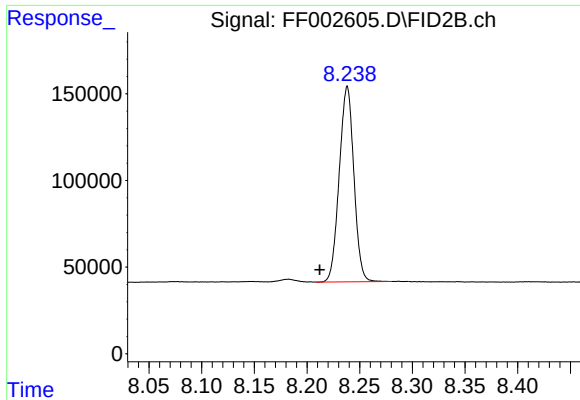


#6 N-TETRADECANE

R.T.: 8.238 min
Delta R.T.: 0.026 min
Response: 1089512
Conc: 9.84 ug/ml

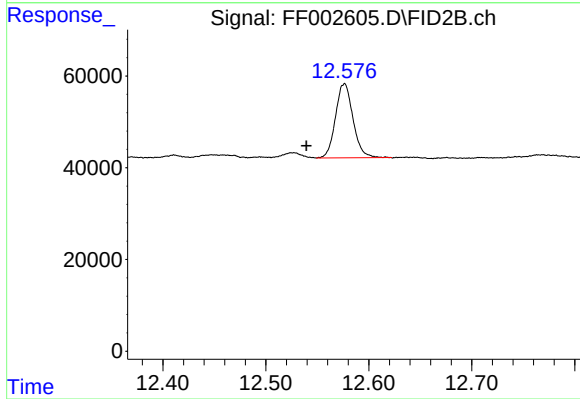


#9 N-EICOSANE

R.T.: 12.576 min
Delta R.T.: 0.037 min
Response: 190796
Conc: 1.71 ug/ml

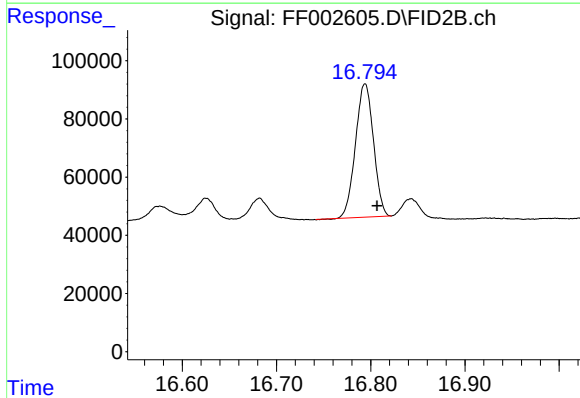


#11 N-OCTACOSANE

R.T.: 16.794 min
Delta R.T.: -0.013 min
Response: 608122
Conc: 5.82 ug/ml

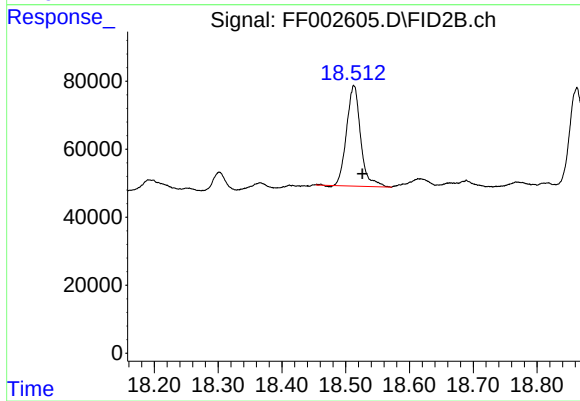

#12 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: -0.014 min
Response: 453988
Conc: 4.77 ug/ml

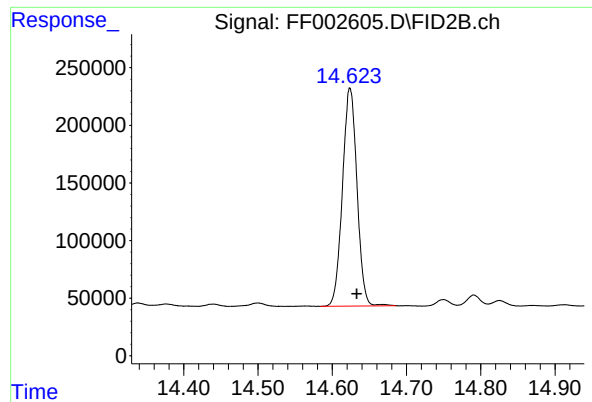

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.624 min
Delta R.T.: -0.009 min
Response: 2571279
Conc: 20.49 ug/ml