

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110618\
 Data File : FF002615.D
 Signal(s) : FID2B.ch
 Acq On : 07 Nov 2018 12:44
 Operator : AJ\SJ
 Sample : J5827-39
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 16:03:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
 Quant Title :
 QLast Update : Wed Nov 07 09:33:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.626	1625736	12.953 ug/ml
Target Compounds			
6) N-TETRADECANE	8.240	815237	7.359 ug/ml
9) N-EICOSANE	12.581	591163	5.300 ug/ml
10) N-TETRACOSANE	14.795	449449	4.194 ug/ml
11) N-OCTACOSANE	16.798	682710	6.537 ug/ml
12) N-DOTRIACONTANE	18.519	588150	6.185 ug/ml
14) N-HEXATRIACONTANE	20.049	204257	2.812 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110618\
Data File : FF002615.D
Signal(s) : FID2B.ch
Acq On : 07 Nov 2018 12:44
Operator : AJ\SJ
Sample : J5827-39
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 16:03:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

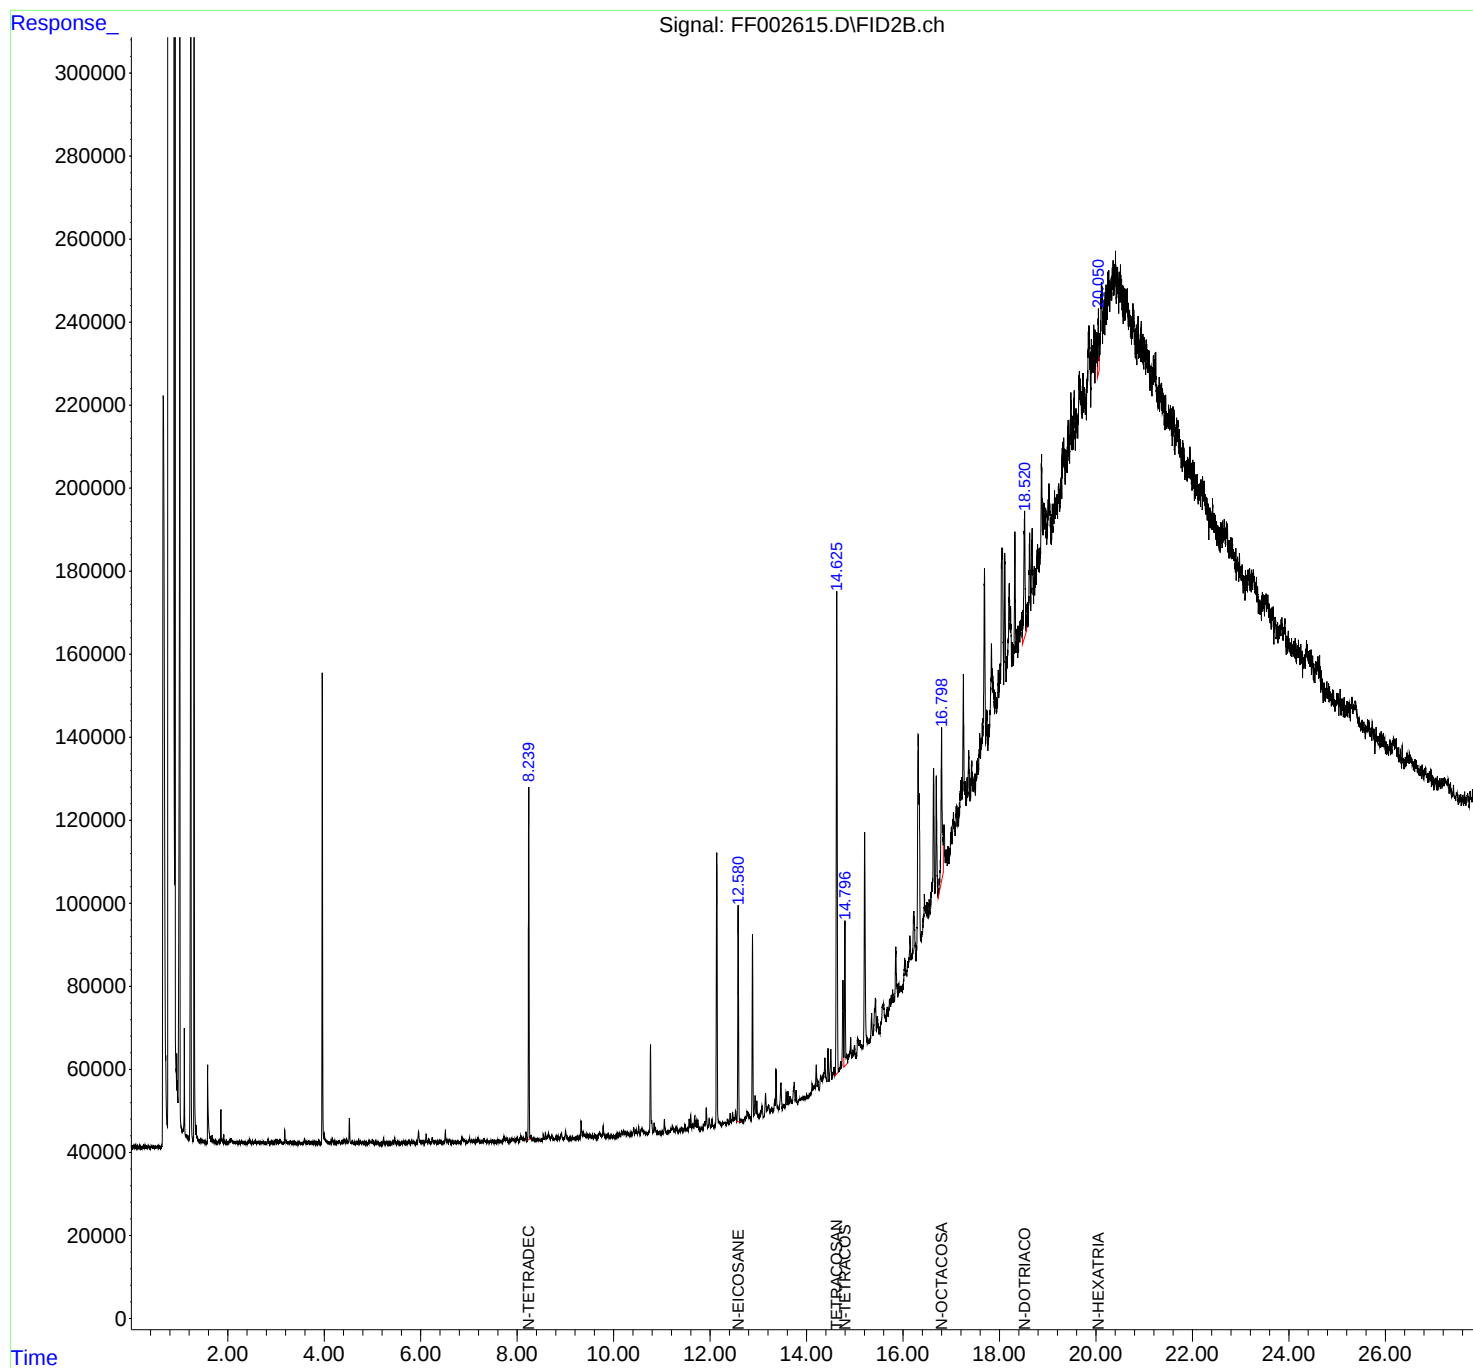

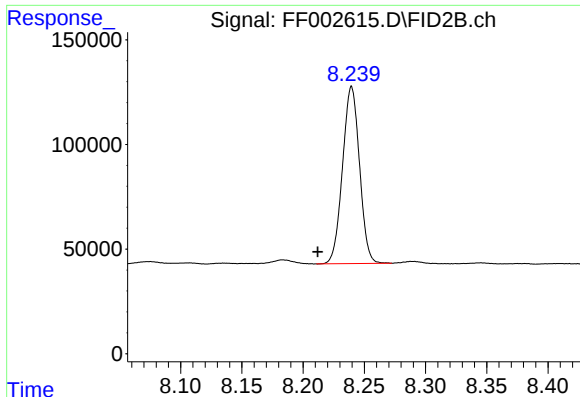


#6 N-TETRADECANE

R.T.: 8.240 min
Delta R.T.: 0.028 min
Response: 815237
Conc: 7.36 ug/ml

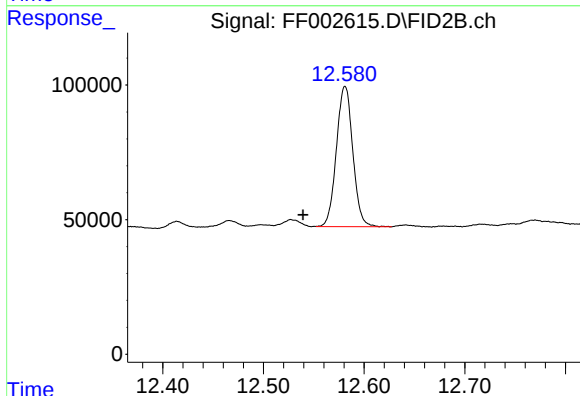


#9 N-EICOSANE

R.T.: 12.581 min
Delta R.T.: 0.042 min
Response: 591163
Conc: 5.30 ug/ml

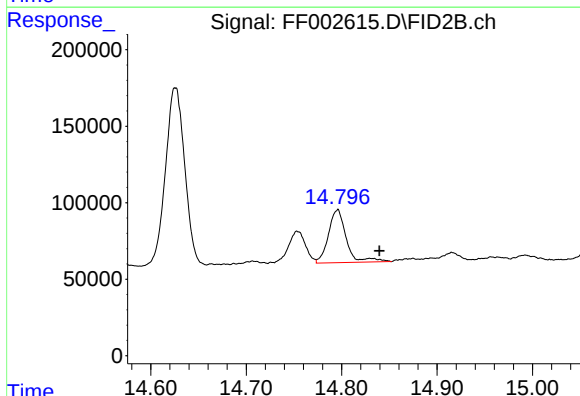


#10 N-TETRACOSANE

R.T.: 14.795 min
Delta R.T.: -0.044 min
Response: 449449
Conc: 4.19 ug/ml

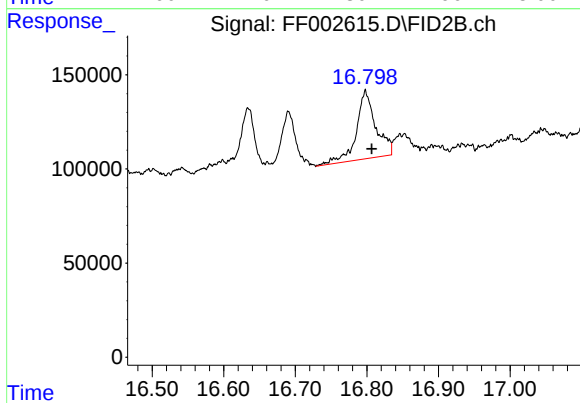


#11 N-OCTACOSANE

R.T.: 16.798 min
Delta R.T.: -0.009 min
Response: 682710
Conc: 6.54 ug/ml

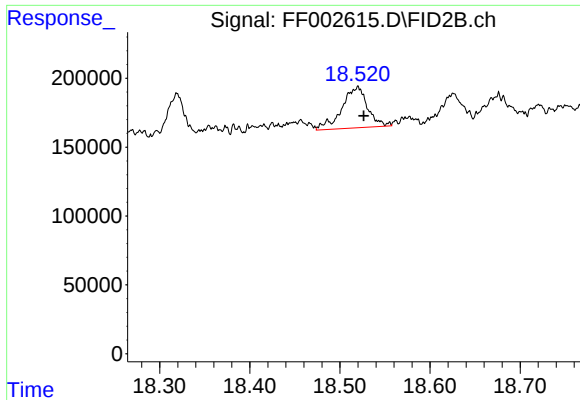


#12 N-DOTRIACONTANE

R.T.: 18.519 min
Delta R.T.: -0.007 min
Response: 588150
Conc: 6.18 ug/ml

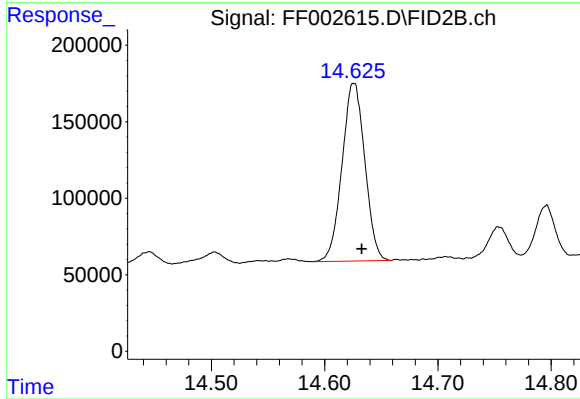

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.626 min
Delta R.T.: -0.007 min
Response: 1625736
Conc: 12.95 ug/ml

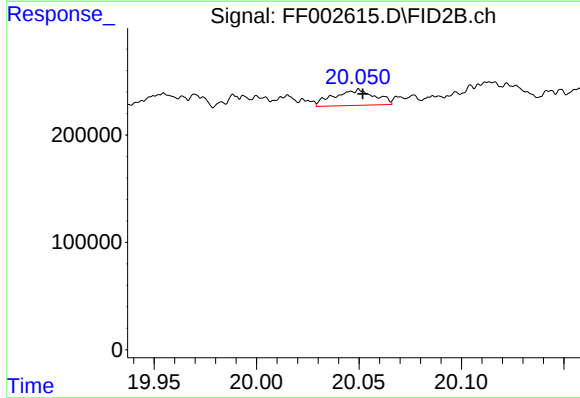

#14 N-HEXATRIACONTANE

R.T.: 20.049 min
Delta R.T.: -0.003 min
Response: 204257
Conc: 2.81 ug/ml