

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110619\
 Data File : FF005934.D
 Signal(s) : FID2B.ch
 Acq On : 06 Nov 2019 17:12
 Operator : DD\AJ
 Sample : K5609-14 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 07 00:36:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	197640	1.759 ug/ml
Target Compounds			
2) N-DECANE	4.407	813387	6.333 ug/ml
3) N-DODECANE	6.422	1136871	8.736 ug/ml
4) N-TETRADECANE	8.213	1527929	11.723 ug/ml
5) N-HEXADECANE	9.810	1774276	13.473 ug/ml
6) N-OCTADECANE	11.248	1425062	10.928 ug/ml
7) N-EICOSANE	12.555	795699	6.069 ug/ml
8) N-DOCOSANE	13.749	350694	2.707 ug/ml
12) N-OCTACOSANE	16.814	143617	1.161 ug/ml
13) N-TRIACONTANE	17.698	282072	2.324 ug/ml
14) N-DOTRIACONTANE	18.530	215777	1.885 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110619\
Data File : FF005934.D
Signal(s) : FID2B.ch
Acq On : 06 Nov 2019 17:12
Operator : DD\AJ
Sample : K5609-14 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 07 00:36:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

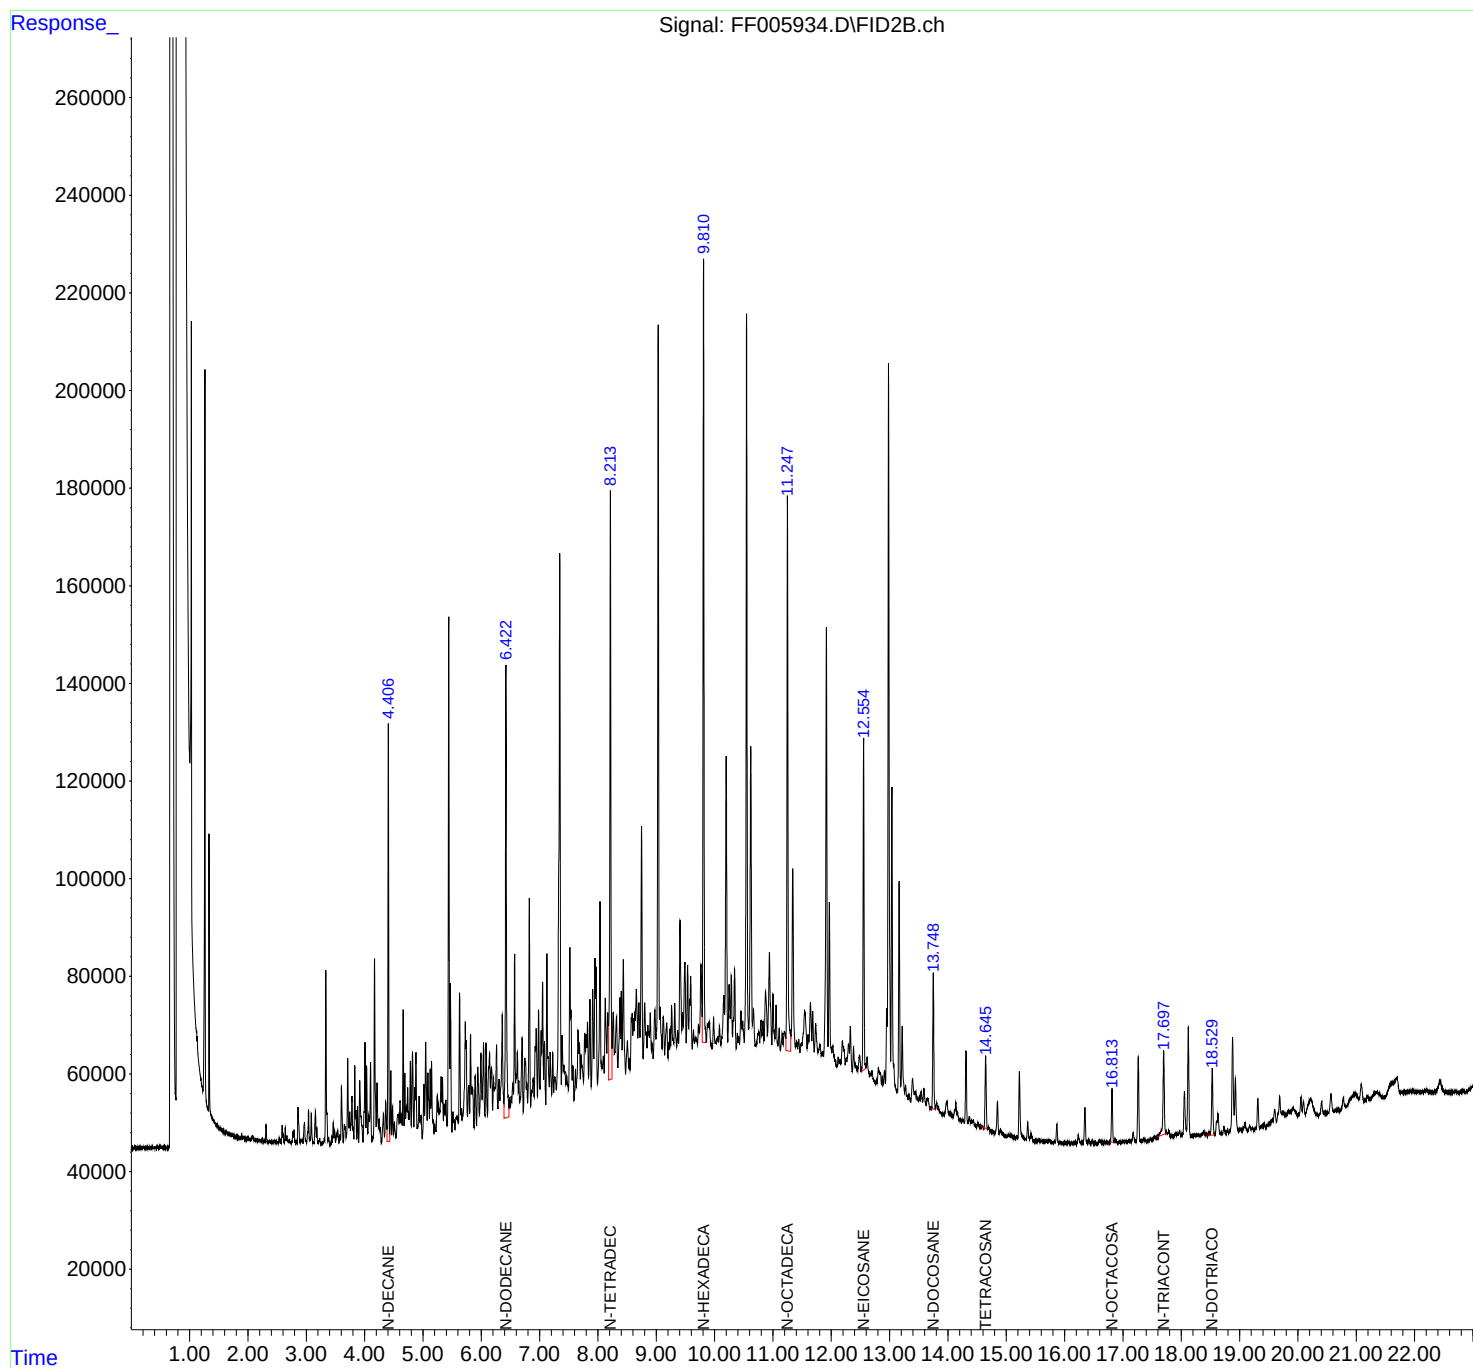


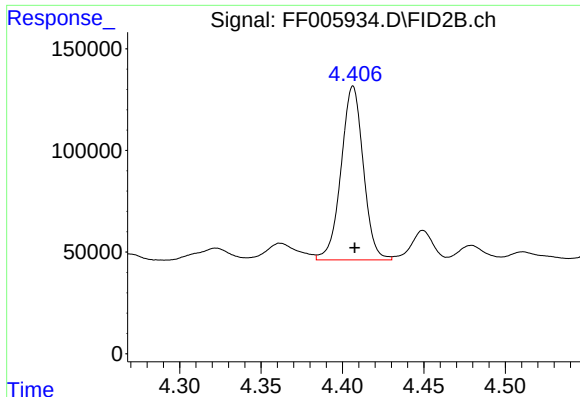

#2 N-DECANE


R.T.: 4.407 min
Delta R.T.: -0.001 min
Response: 813387
Conc: 6.33 ug/ml

Instrument :
FID_F
ClientSampleId :

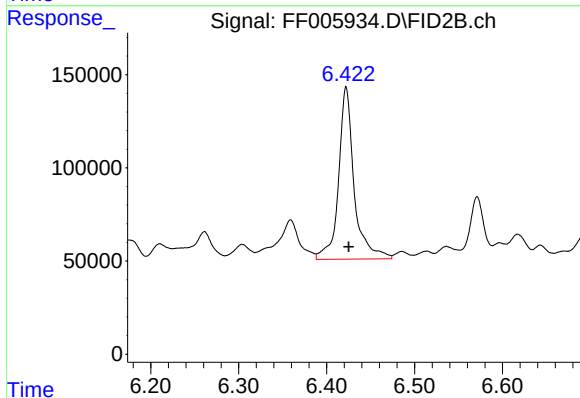


#3 N-DODECANE

R.T.: 6.422 min
Delta R.T.: -0.003 min
Response: 1136871
Conc: 8.74 ug/ml

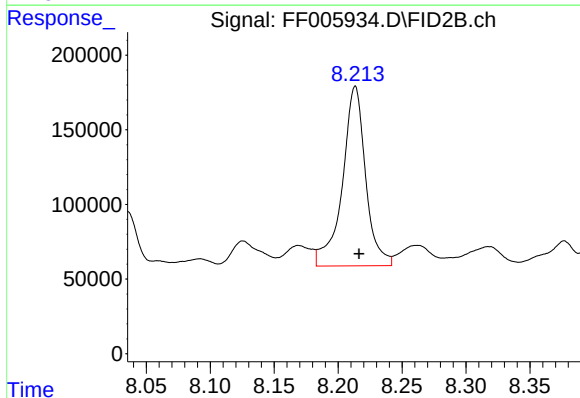


#4 N-TETRADECANE

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 1527929
Conc: 11.72 ug/ml

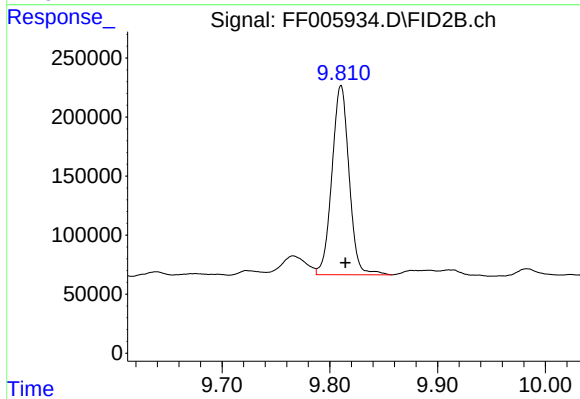

#5 N-HEXADECANE


R.T.: 9.810 min
Delta R.T.: -0.004 min
Response: 1774276
Conc: 13.47 ug/ml

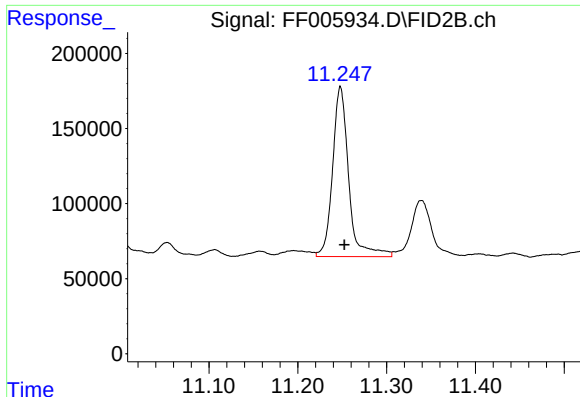

#6 N-OCTADECANE


R.T.: 11.248 min
Delta R.T.: -0.005 min
Response: 1425062
Conc: 10.93 ug/ml

Instrument :
FID_F
ClientSampleId :

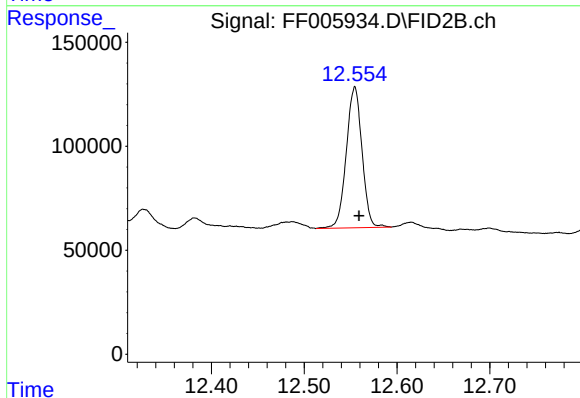


#7 N-EICOSANE

R.T.: 12.555 min
Delta R.T.: -0.004 min
Response: 795699
Conc: 6.07 ug/ml

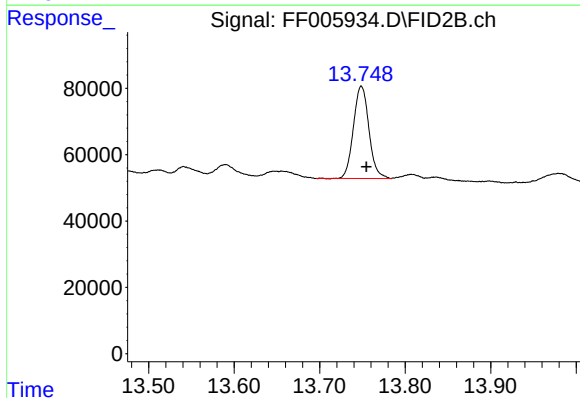


#8 N-DOCOSANE

R.T.: 13.749 min
Delta R.T.: -0.006 min
Response: 350694
Conc: 2.71 ug/ml

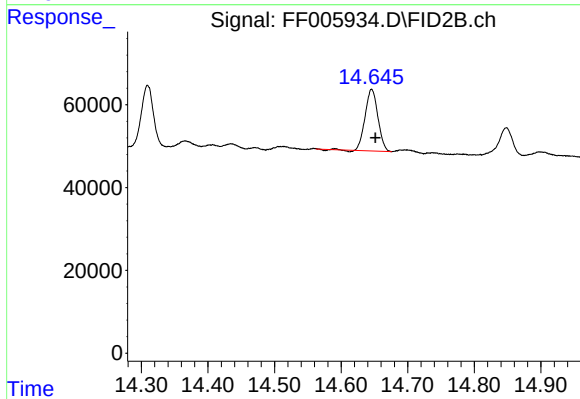

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.646 min
Delta R.T.: -0.006 min
Response: 197640
Conc: 1.76 ug/ml

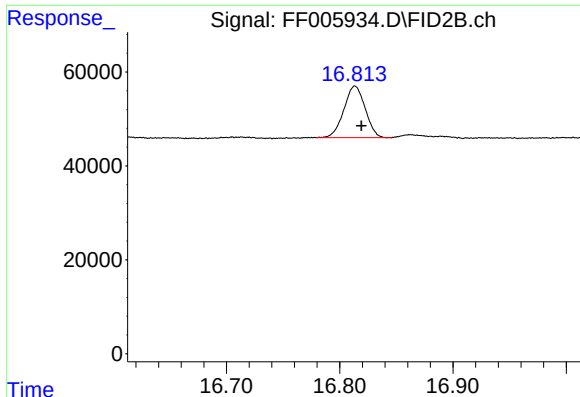

#12 N-OCTACOSANE


R.T.: 16.814 min
Delta R.T.: -0.006 min
Response: 143617
Conc: 1.16 ug/ml

Instrument :
FID_F
ClientSampleId :

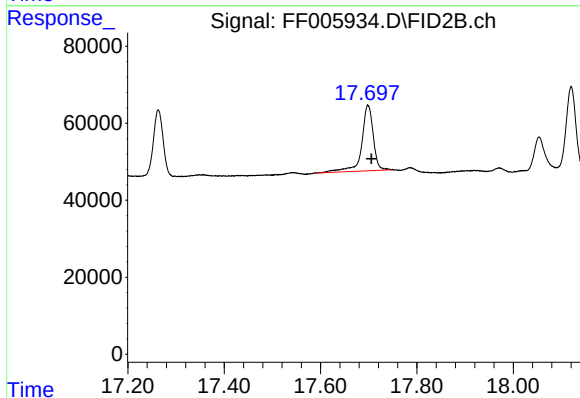

#13 N-TRIACONTANE

R.T.: 17.698 min
Delta R.T.: -0.007 min
Response: 282072
Conc: 2.32 ug/ml

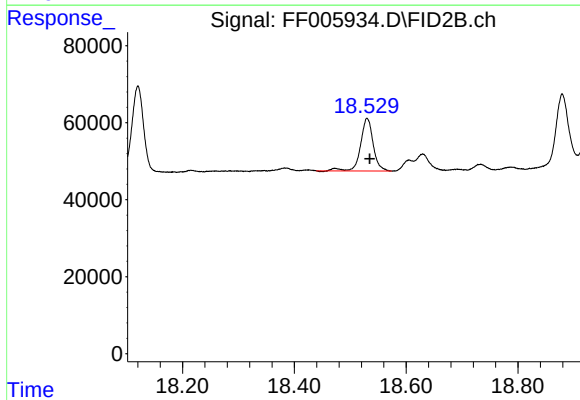

#14 N-DOTRIACONTANE

R.T.: 18.530 min
Delta R.T.: -0.005 min
Response: 215777
Conc: 1.88 ug/ml