

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110619\
Data File : FF005935.D
Signal(s) : FID2B.ch
Acq On : 06 Nov 2019 17:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 07 00:37:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	2534019	22.547 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.698	123160	1.015 ug/ml
14) N-DOTRIACONTANE	18.530	172129	1.504 ug/ml
16) N-HEXATRIACONTANE	20.093	163673	1.629 ug/ml
18) N-TETRACONTANE	21.699	274967	3.072 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110619\
Data File : FF005935.D
Signal(s) : FID2B.ch
Acq On : 06 Nov 2019 17:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 07 00:37:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

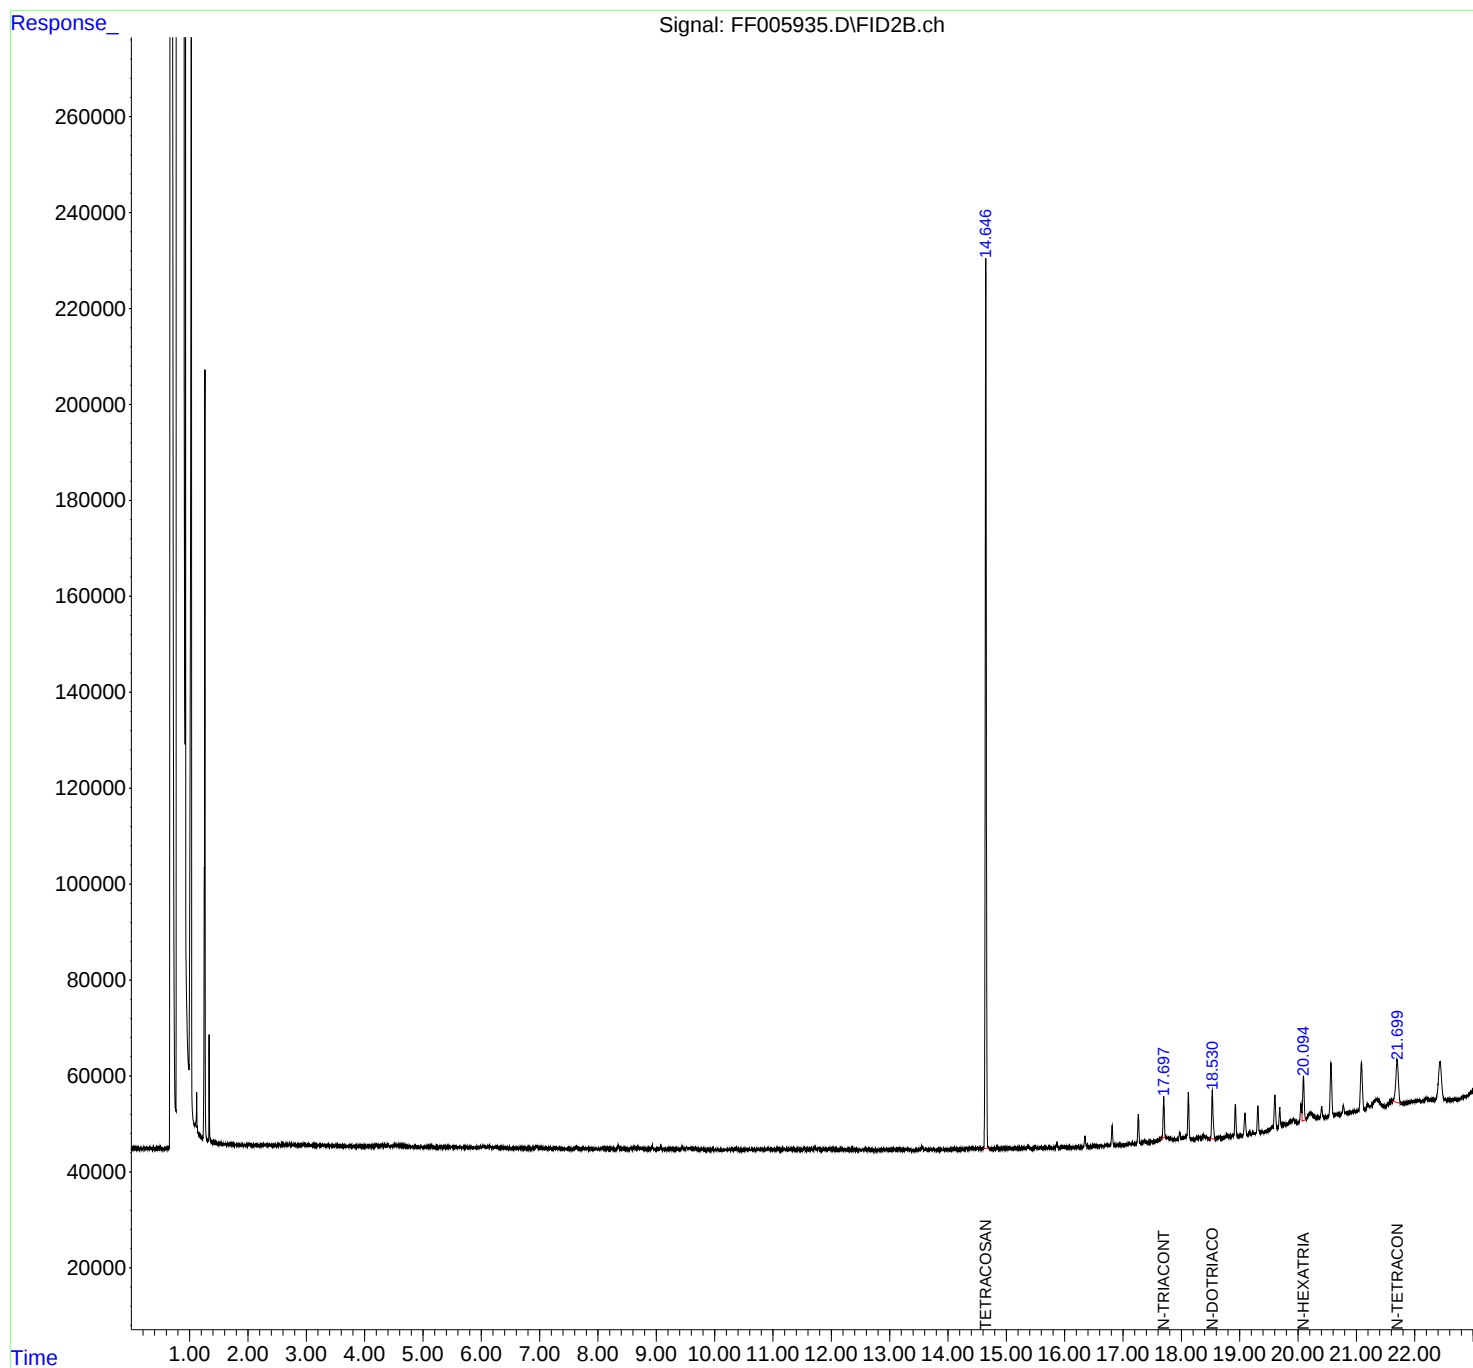


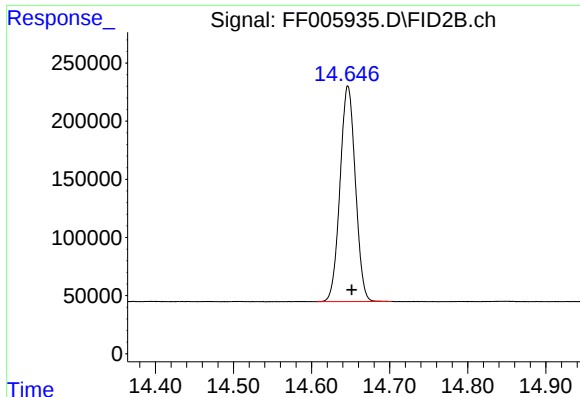

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.647 min
Delta R.T.: -0.005 min
Response: 2534019
Conc: 22.55 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

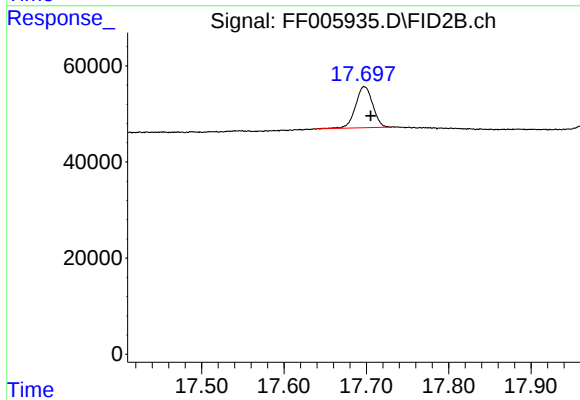


#13 N-TRIACONTANE

R.T.: 17.698 min
Delta R.T.: -0.008 min
Response: 123160
Conc: 1.01 ug/ml

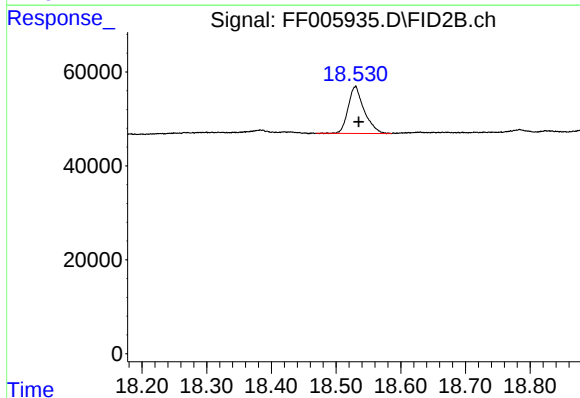


#14 N-DOTRIACONTANE

R.T.: 18.530 min
Delta R.T.: -0.005 min
Response: 172129
Conc: 1.50 ug/ml

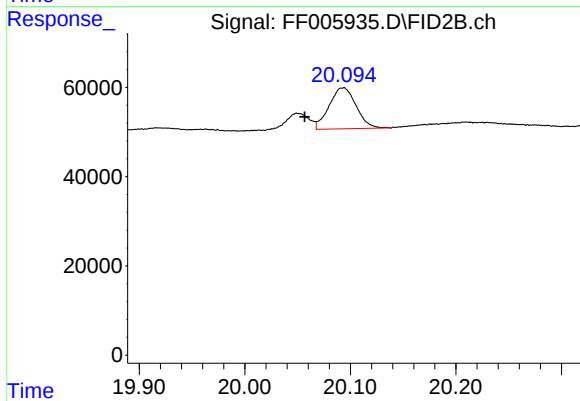

#16 N-HEXATRIACONTANE

R.T.: 20.093 min
Delta R.T.: 0.036 min
Response: 163673
Conc: 1.63 ug/ml

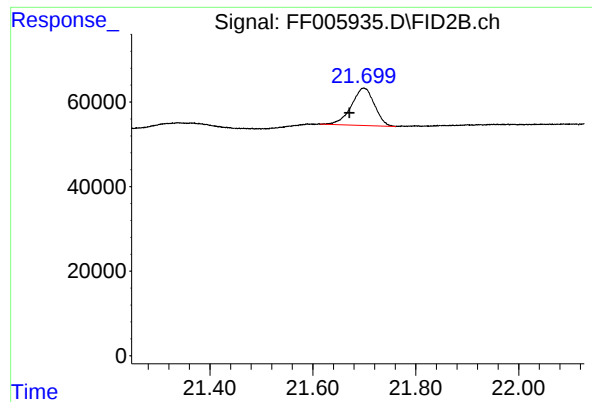

#18 N-TETRACONTANE

R.T.: 21.699 min
Delta R.T.: 0.028 min
Response: 274967
Conc: 3.07 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK