

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110619\
Data File : FF005934.D
Signal(s) : FID2B.ch
Acq On : 06 Nov 2019 17:12
Operator : DD\AJ
Sample : K5676-01MSD
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SU-02-110119MSD

Manual Integrations
APPROVED

Ankita
11/7/2019 11:06:14 AM

Integration File: autoint1.e
Quant Time: Nov 07 00:36:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.645	207191	1.844 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110619\
Data File : FF005934.D
Signal(s) : FID2B.ch
Acq On : 06 Nov 2019 17:12
Operator : DD\AJ
Sample : K5676-01MSD
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SU-02-110119MSD


Manual Integrations
APPROVED

Ankita
11/7/2019 11:06:14 AM

Integration File: autoint1.e
Quant Time: Nov 07 00:36:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

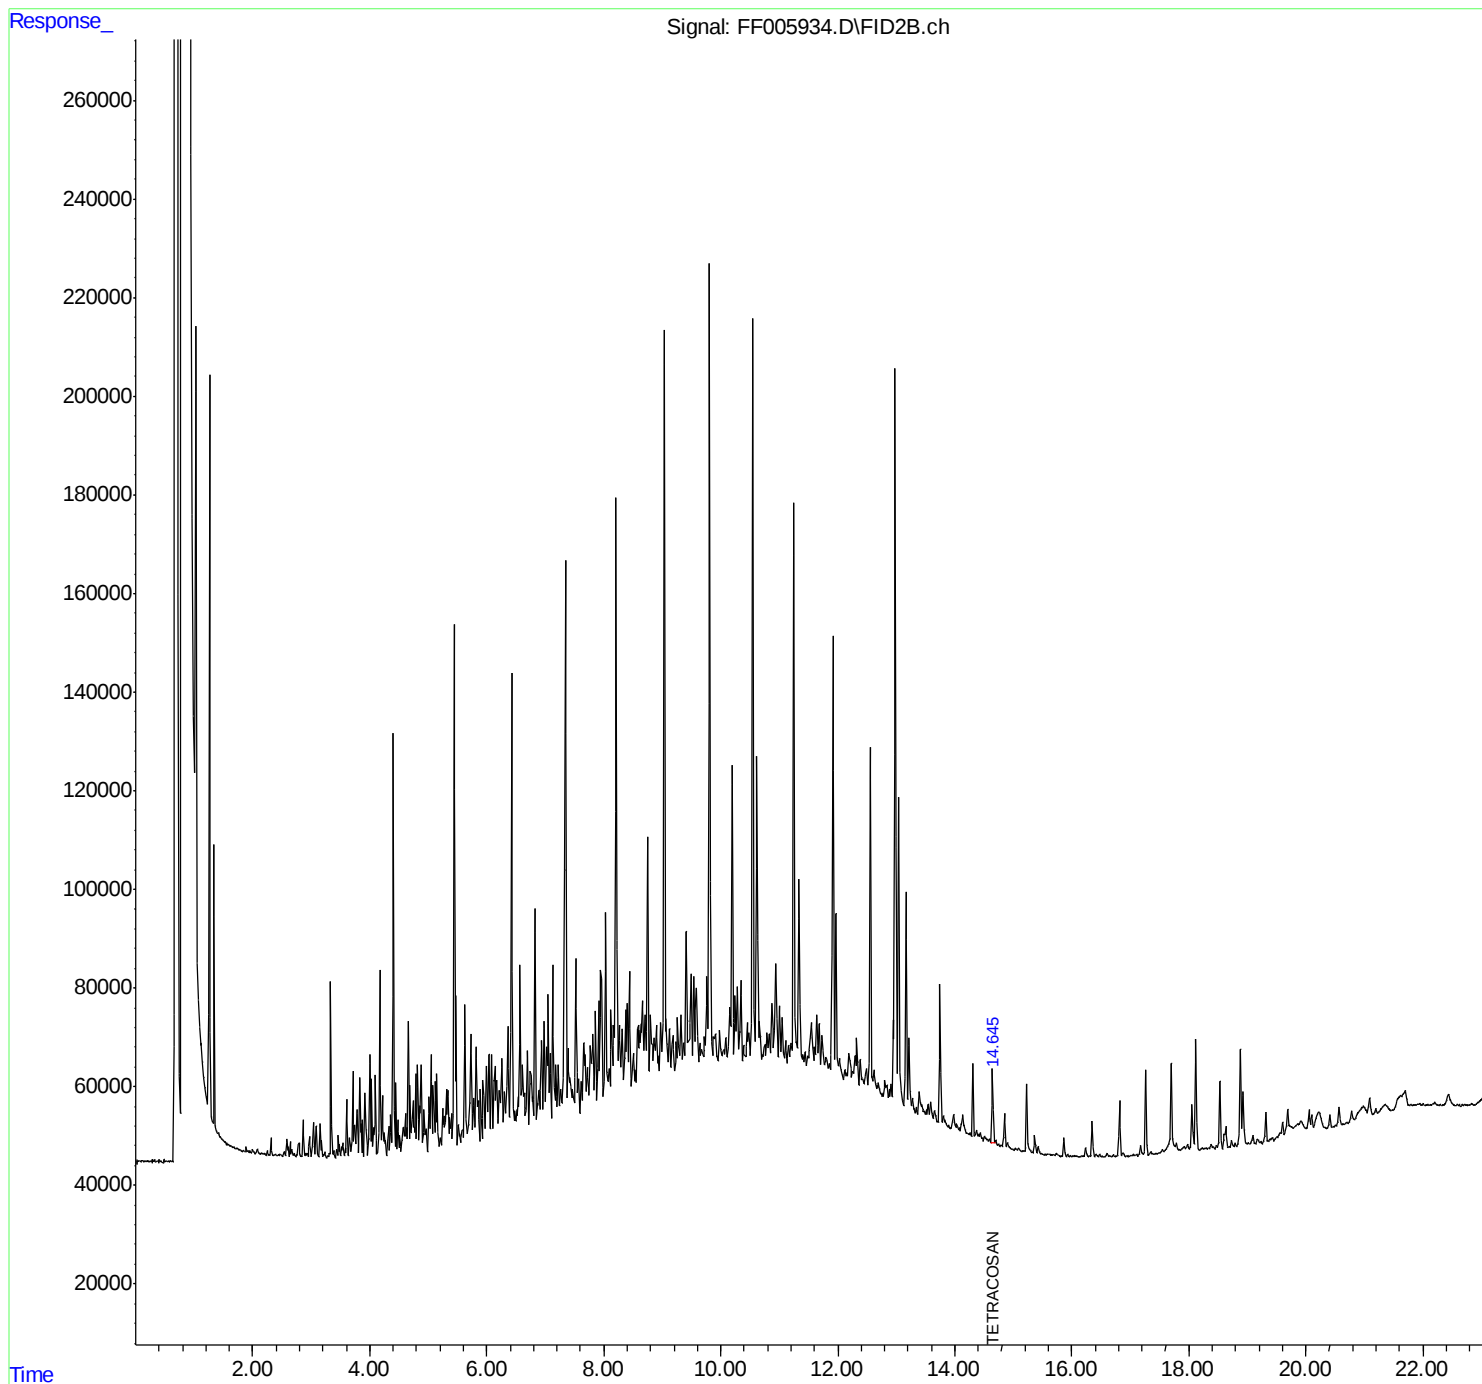

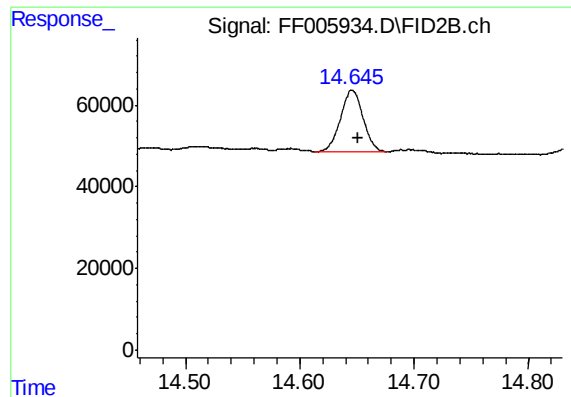

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.645 min
Delta R.T.: -0.006 min
Response: 207191
Conc: 1.84 ug/ml m

Instrument :
FID_F
ClientSampleId :
SU-02-110119MSD

Manual Integrations
APPROVED

Ankita
11/7/2019 11:06:14 AM