

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
Data File : FF002621.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2018 10:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 08 14:25:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.627	2942018	23.440 ug/ml
Target Compounds				
12)	N-DOTRIACONTANE	18.516	268429	2.823 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
Data File : FF002621.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2018 10:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 08 14:25:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

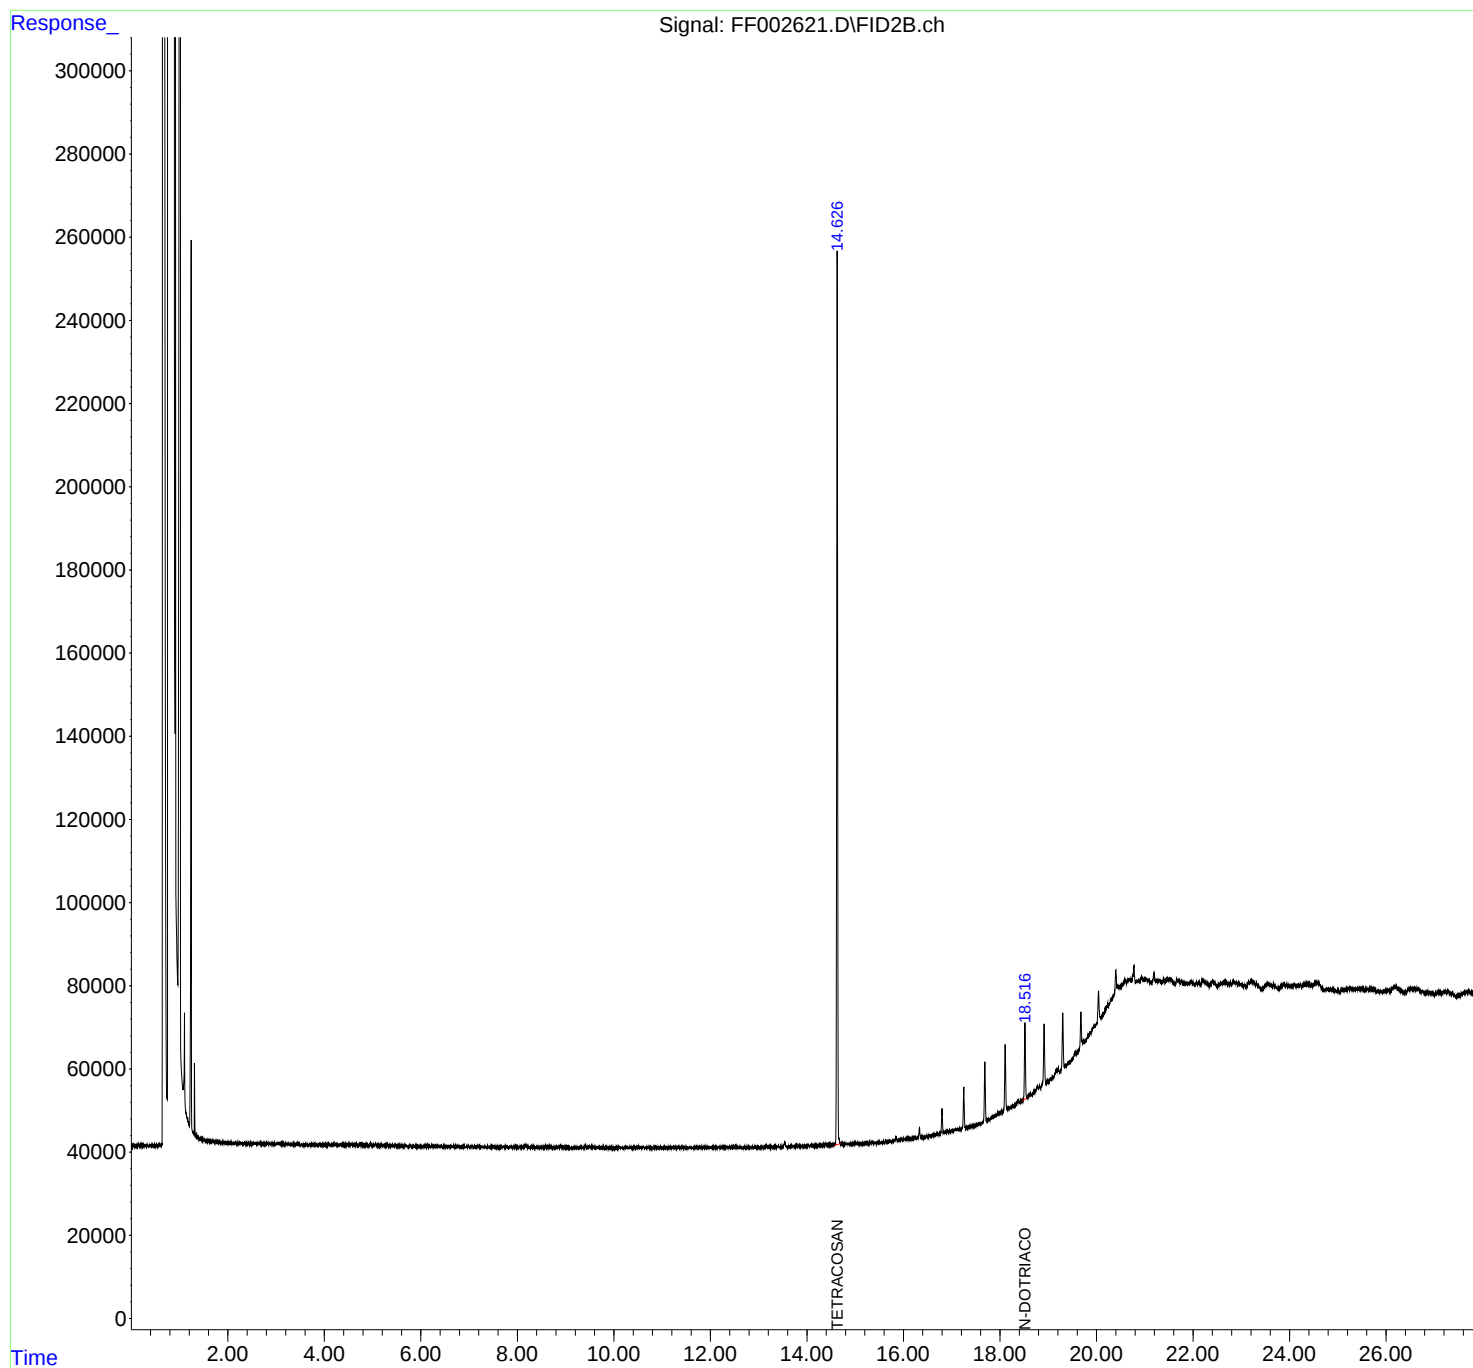

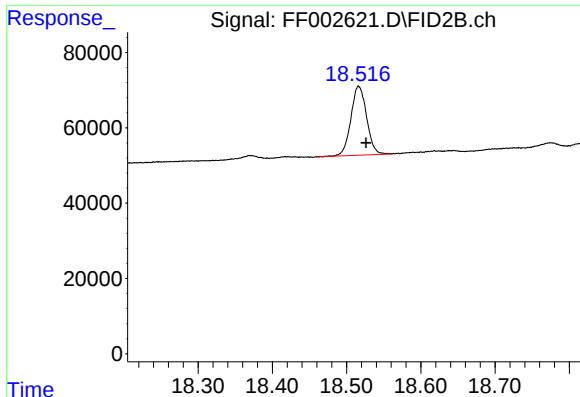

#12 N-DOTRIACONTANE

R.T.: 18.516 min
Delta R.T.: -0.010 min
Response: 268429
Conc: 2.82 ug/ml

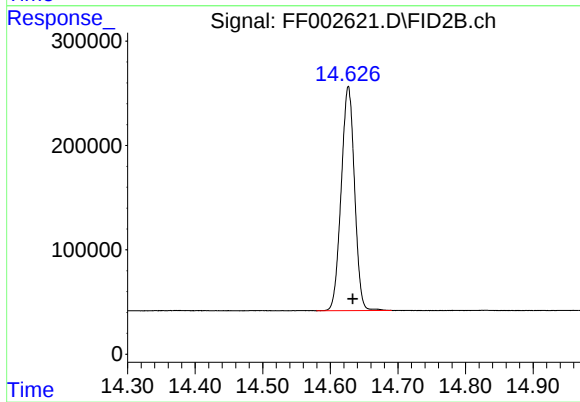

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.006 min
Response: 2942018
Conc: 23.44 ug/ml