

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
 Data File : FF002625.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2018 12:19
 Operator : AJ\SJ
 Sample : J5827-33
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 08 14:26:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
 Quant Title :
 QLast Update : Wed Nov 07 09:33:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.628	2047396	16.312 ug/ml
Target Compounds			
6) N-TETRADECANE	8.240	948935	8.566 ug/ml
9) N-EICOSANE	12.583	1299954	11.655 ug/ml
10) N-TETRACOSANE	14.799	783306	7.310 ug/ml
11) N-OCTACOSANE	16.800	905460	8.670 ug/ml
12) N-DOTRIACONTANE	18.519	752751	7.916 ug/ml
14) N-HEXATRIACONTANE	20.049	210981	2.905 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
Data File : FF002625.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2018 12:19
Operator : AJ\SJ
Sample : J5827-33
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 08 14:26:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

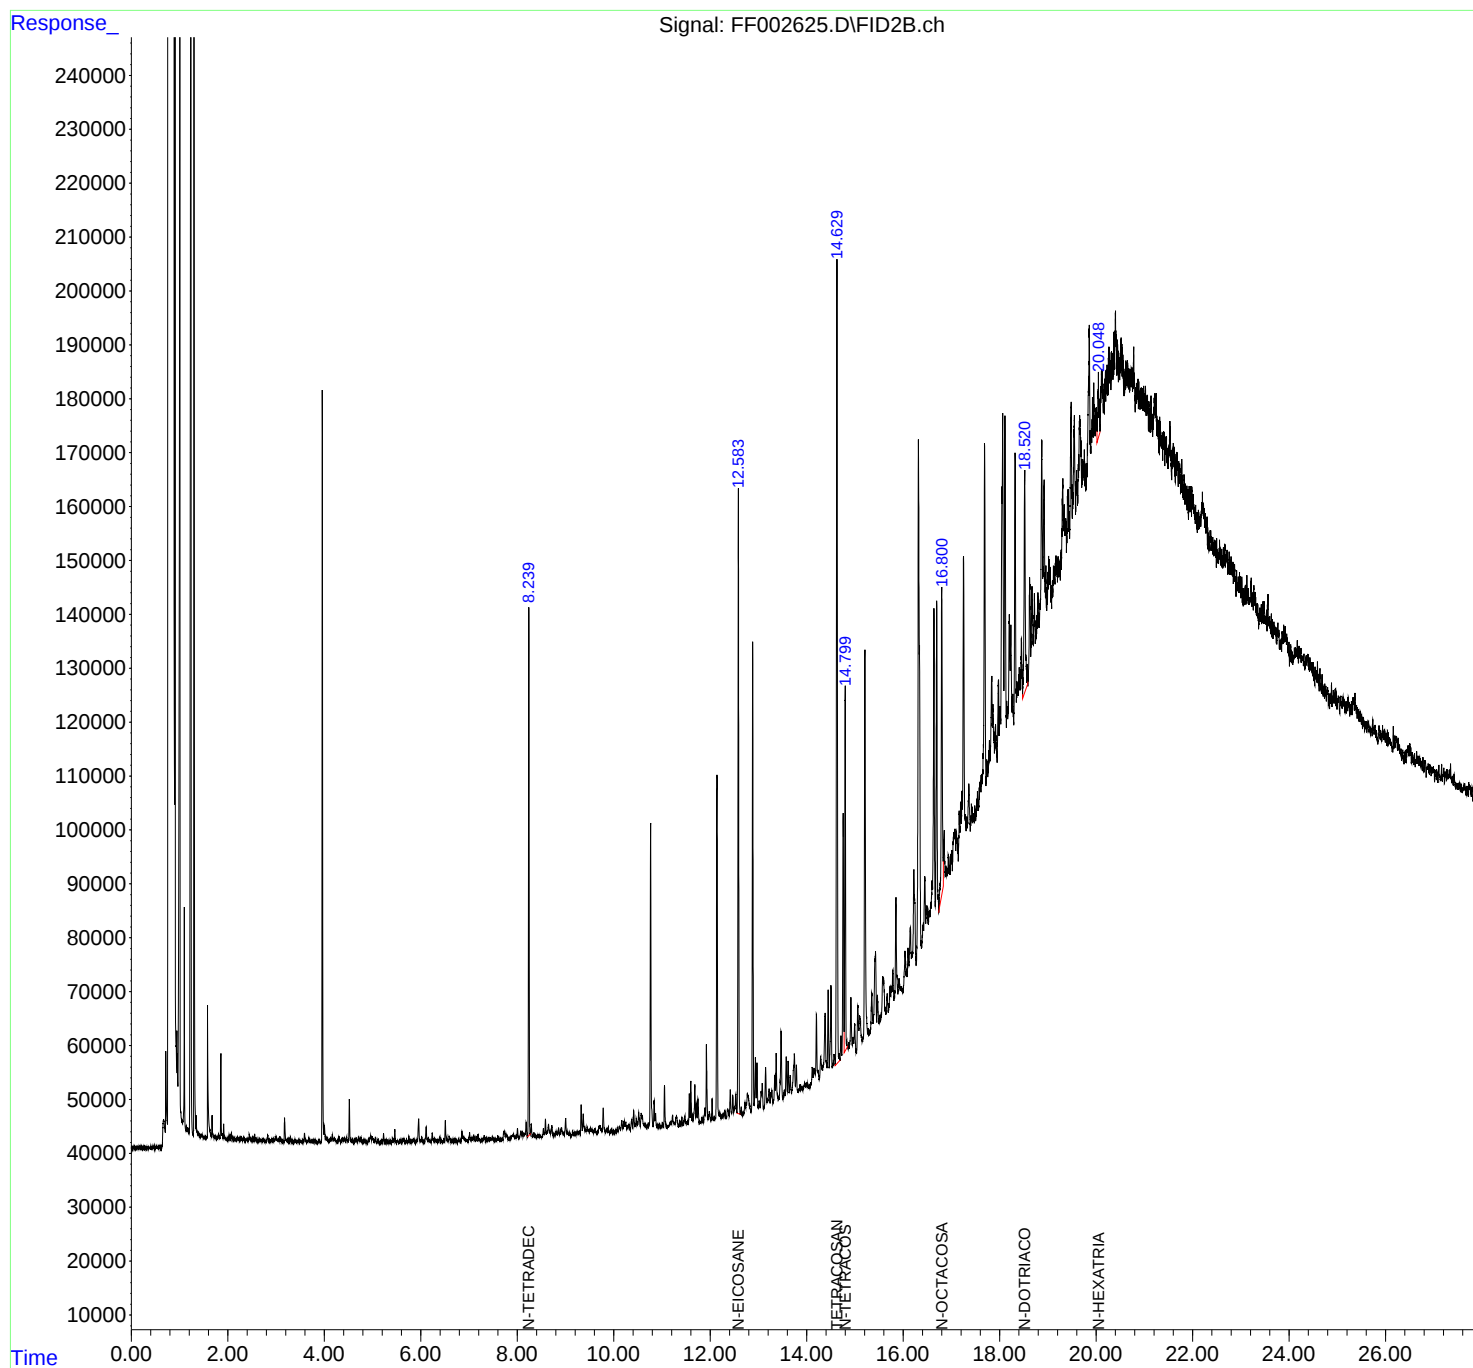

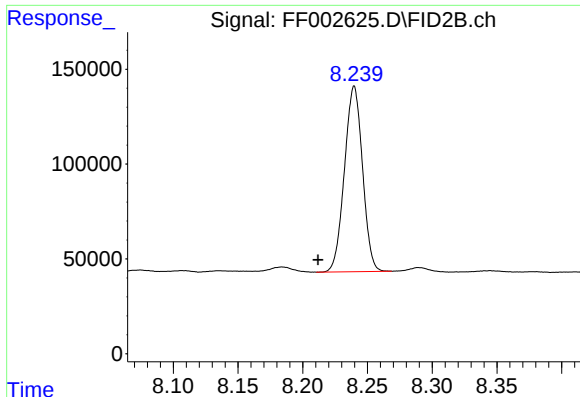


#6 N-TETRADECANE

R.T.: 8.240 min
Delta R.T.: 0.028 min
Response: 948935
Conc: 8.57 ug/ml

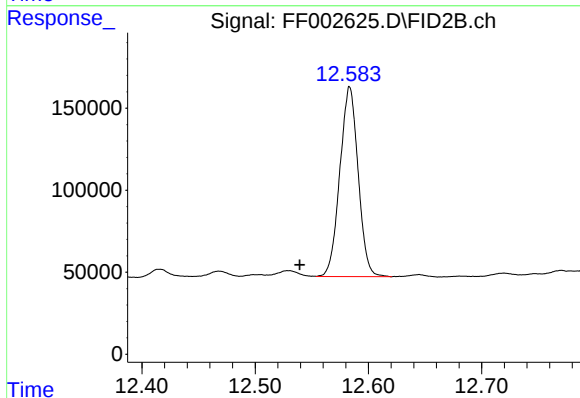


#9 N-EICOSANE

R.T.: 12.583 min
Delta R.T.: 0.044 min
Response: 1299954
Conc: 11.65 ug/ml

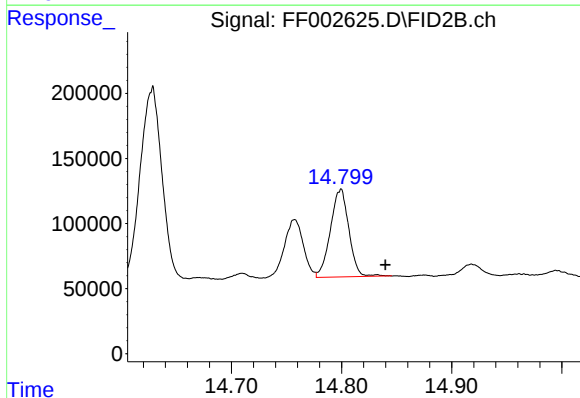


#10 N-TETRACOSANE

R.T.: 14.799 min
Delta R.T.: -0.041 min
Response: 783306
Conc: 7.31 ug/ml

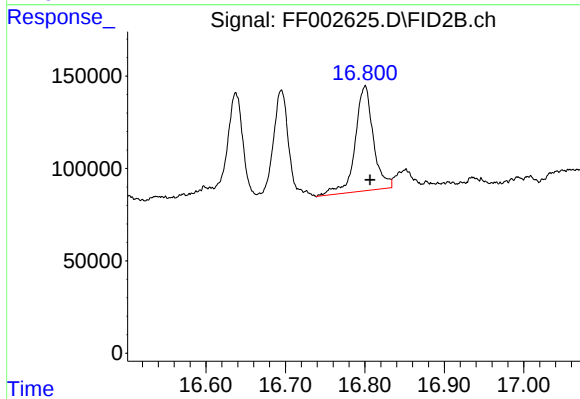


#11 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: -0.007 min
Response: 905460
Conc: 8.67 ug/ml

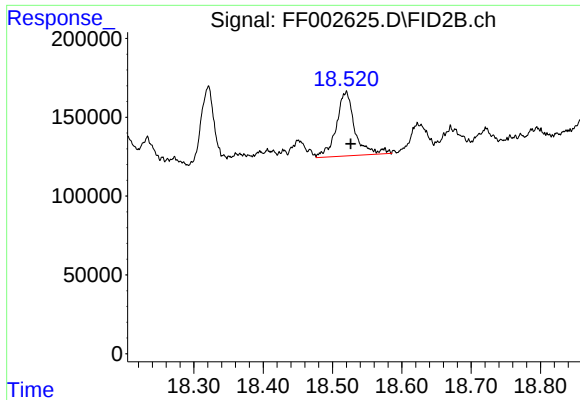


#12 N-DOTRIACONTANE

R.T.: 18.519 min
Delta R.T.: -0.007 min
Response: 752751
Conc: 7.92 ug/ml

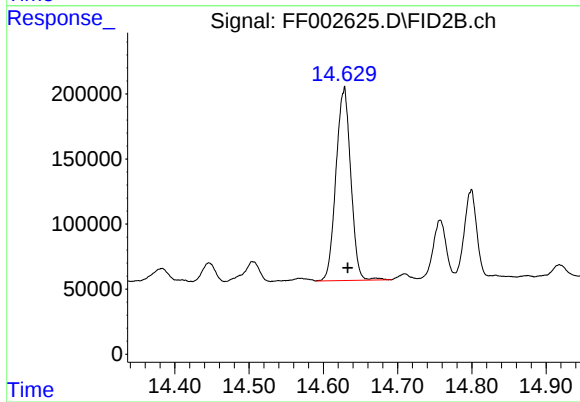

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.628 min
Delta R.T.: -0.005 min
Response: 2047396
Conc: 16.31 ug/ml

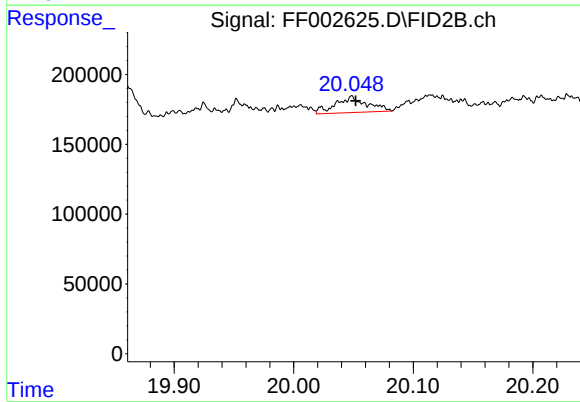

#14 N-HEXATRIACONTANE

R.T.: 20.049 min
Delta R.T.: -0.003 min
Response: 210981
Conc: 2.90 ug/ml