

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
 Data File : FF002626.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2018 12:54
 Operator : AJ\SJ
 Sample : J5827-28 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 08 14:26:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
 Quant Title :
 QLast Update : Wed Nov 07 09:33:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.626	432583	3.447 ug/ml
Target Compounds			
6) N-TETRADECANE	8.239	184170	1.663 ug/ml
9) N-EICOSANE	12.582	509471	4.568 ug/ml
10) N-TETRACOSANE	14.797	295432	2.757 ug/ml
11) N-OCTACOSANE	16.799	169341	1.621 ug/ml
12) N-DOTRIACONTANE	18.518	386312	4.062 ug/ml
14) N-HEXATRIACONTANE	20.050	351770	4.843 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
Data File : FF002626.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2018 12:54
Operator : AJ\SJ
Sample : J5827-28 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 08 14:26:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

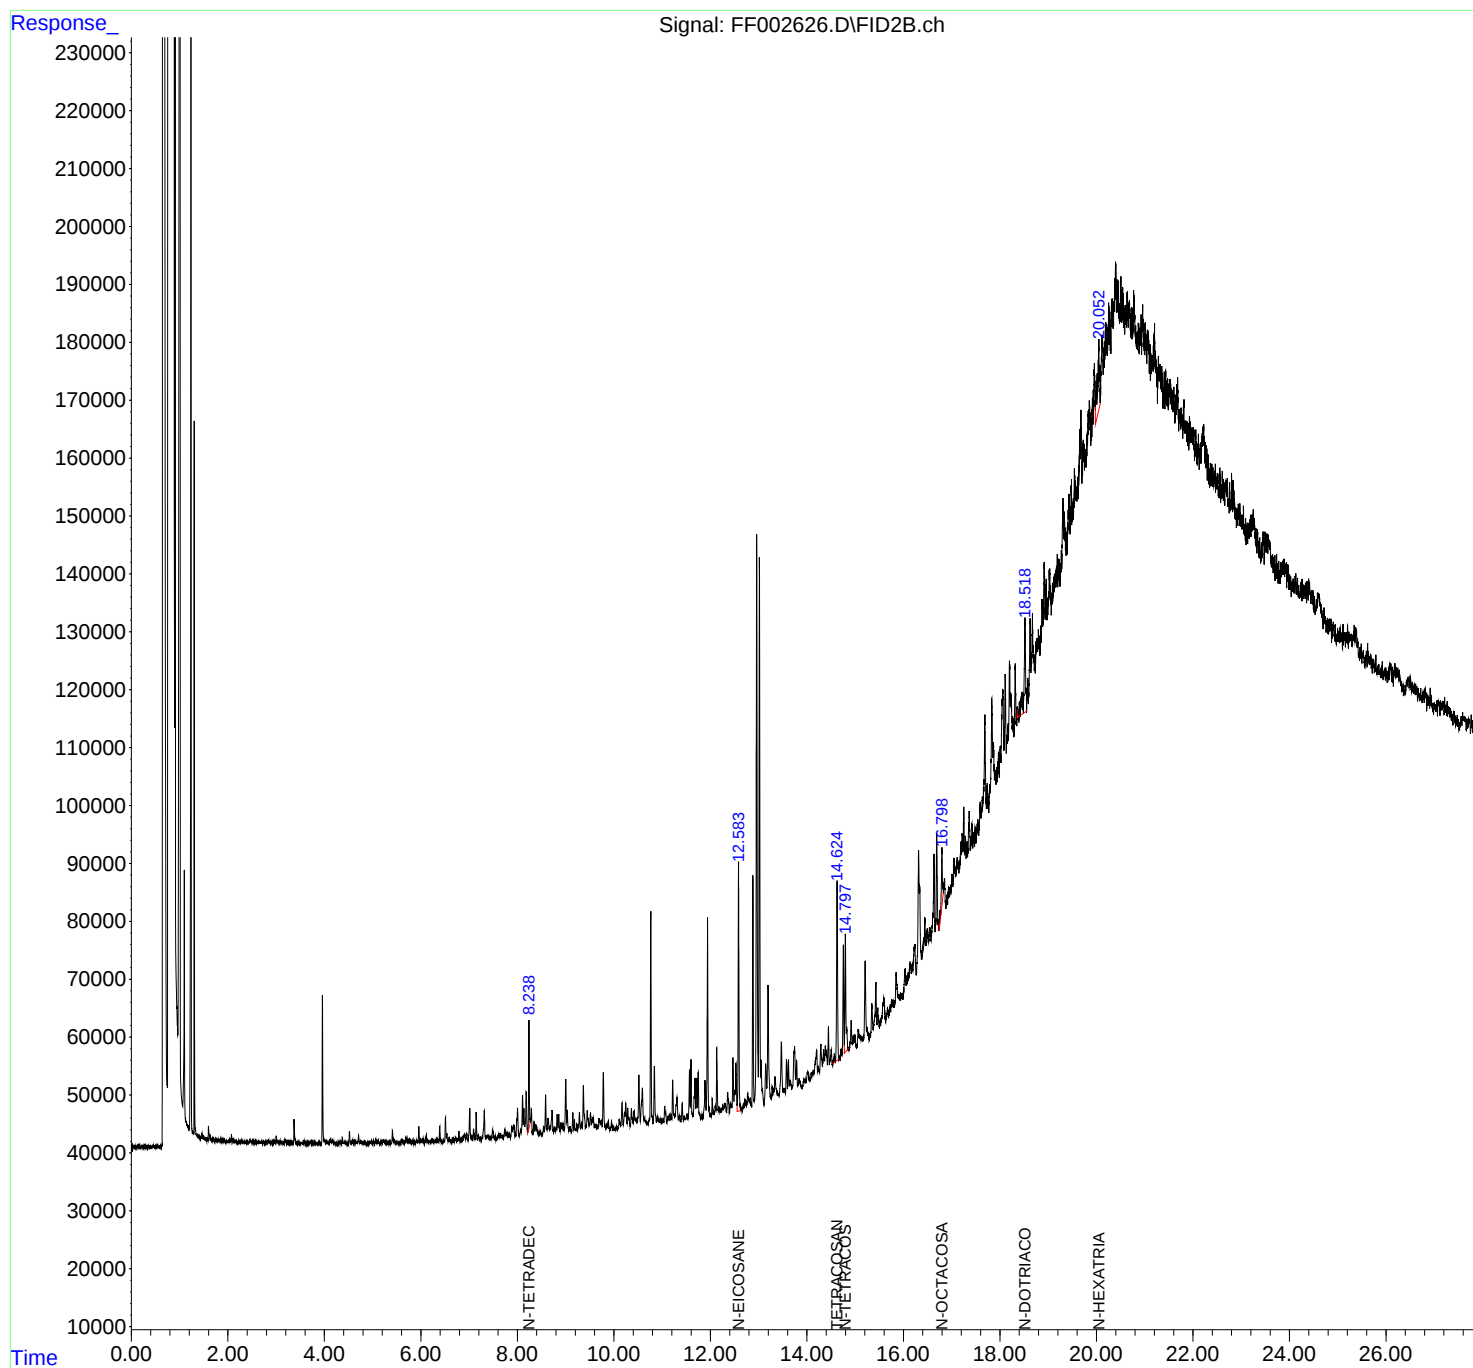

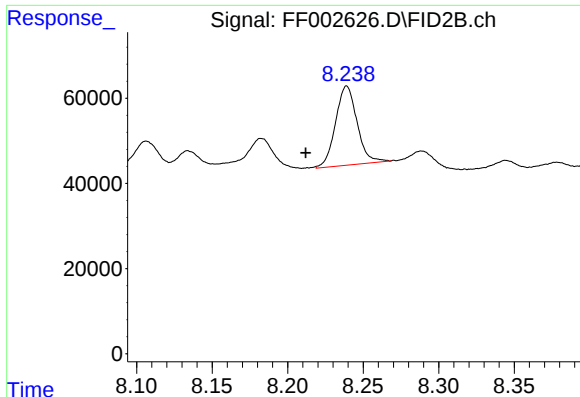


#6 N-TETRADECANE

R.T.: 8.239 min
Delta R.T.: 0.027 min
Response: 184170
Conc: 1.66 ug/ml

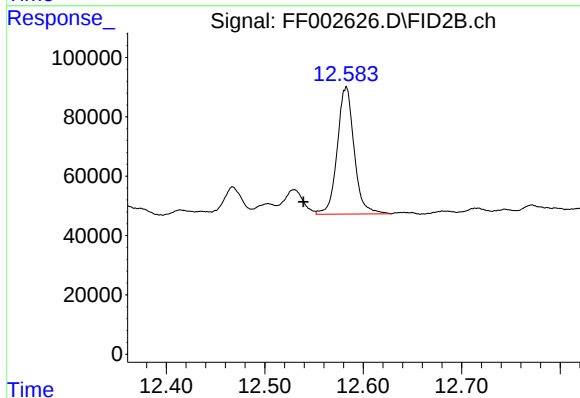


#9 N-EICOSANE

R.T.: 12.582 min
Delta R.T.: 0.043 min
Response: 509471
Conc: 4.57 ug/ml

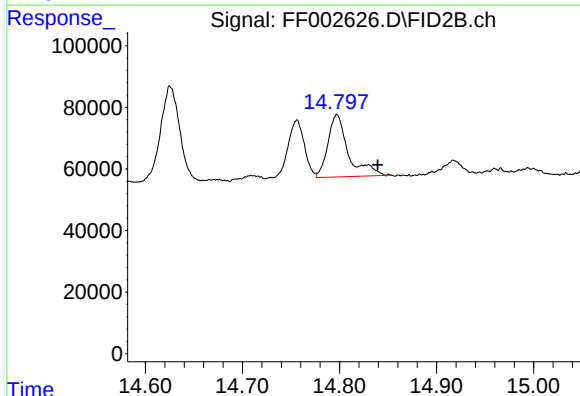


#10 N-TETRACOSANE

R.T.: 14.797 min
Delta R.T.: -0.042 min
Response: 295432
Conc: 2.76 ug/ml

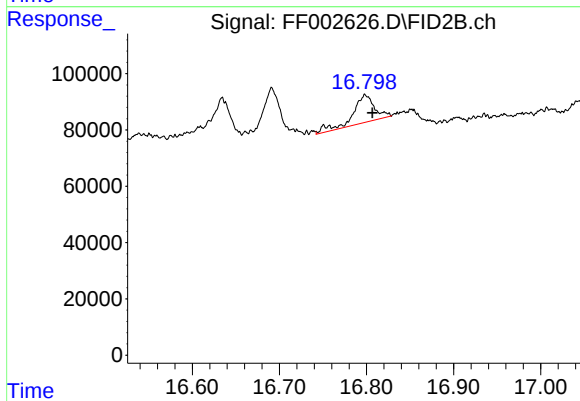


#11 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: -0.008 min
Response: 169341
Conc: 1.62 ug/ml

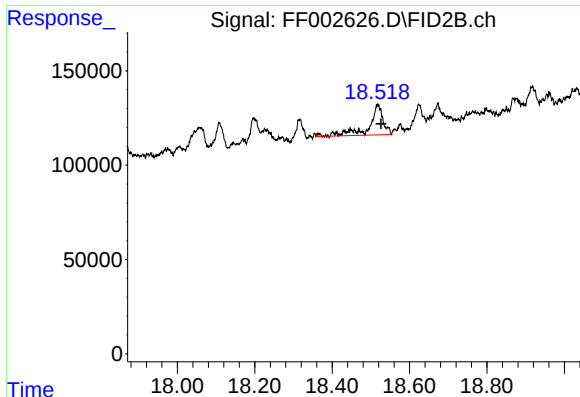


#12 N-DOTRIACONTANE

R.T.: 18.518 min
Delta R.T.: -0.008 min
Response: 386312
Conc: 4.06 ug/ml

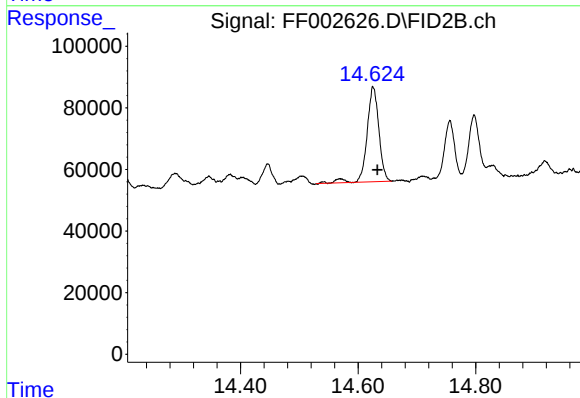

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.626 min
Delta R.T.: -0.007 min
Response: 432583
Conc: 3.45 ug/ml

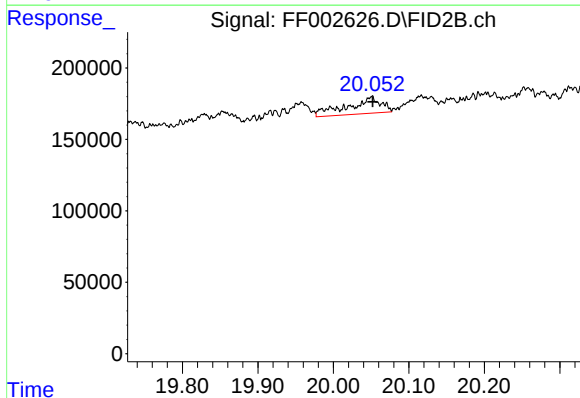

#14 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: -0.002 min
Response: 351770
Conc: 4.84 ug/ml