

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
 Data File : FF002628.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2018 14:04
 Operator : AJ\SJ
 Sample : J5827-27 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 08 14:32:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
 Quant Title :
 QLast Update : Wed Nov 07 09:33:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.627	446275	3.556 ug/ml
Target Compounds				
6)	N-TETRADECANE	8.239	196895	1.777 ug/ml
7)	N-HEXADECANE	9.785	175660	1.559 ug/ml
9)	N-EICOSANE	12.585	1630551	14.619 ug/ml
10)	N-TETRACOSANE	14.799	744549	6.948 ug/ml
11)	N-OCTACOSANE	16.799	235708	2.257 ug/ml
12)	N-DOTRIACONTANE	18.521	299848	3.153 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110818\
Data File : FF002628.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2018 14:04
Operator : AJ\SJ
Sample : J5827-27 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 08 14:32:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF110618.M
Quant Title :
QLast Update : Wed Nov 07 09:33:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

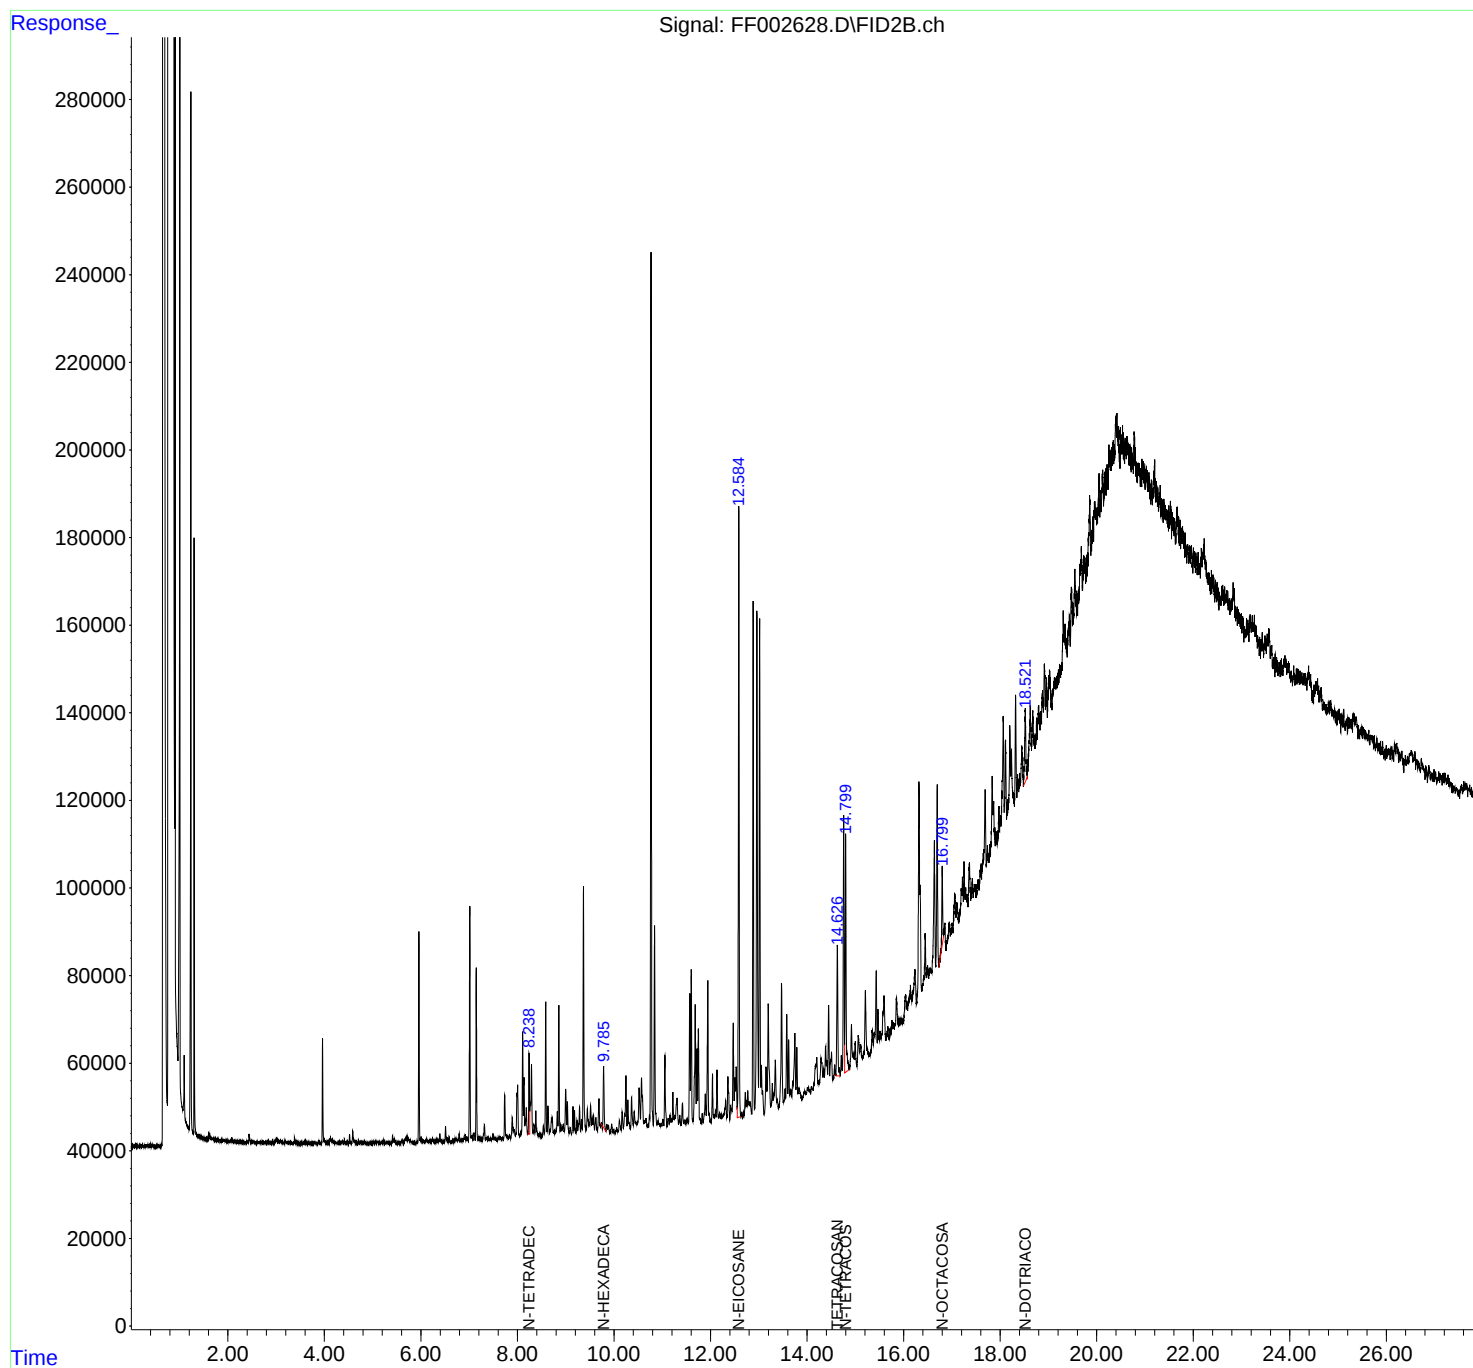

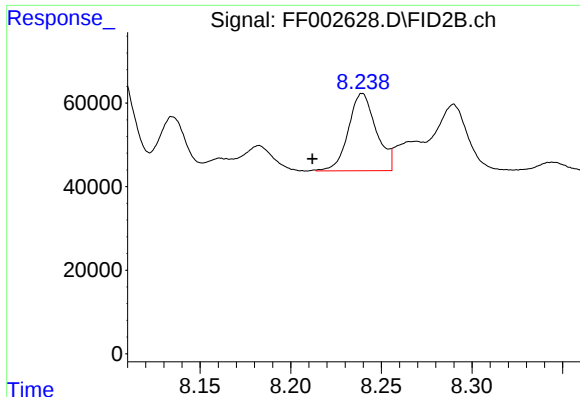


#6 N-TETRADECANE

R.T.: 8.239 min
Delta R.T.: 0.028 min
Response: 196895
Conc: 1.78 ug/ml

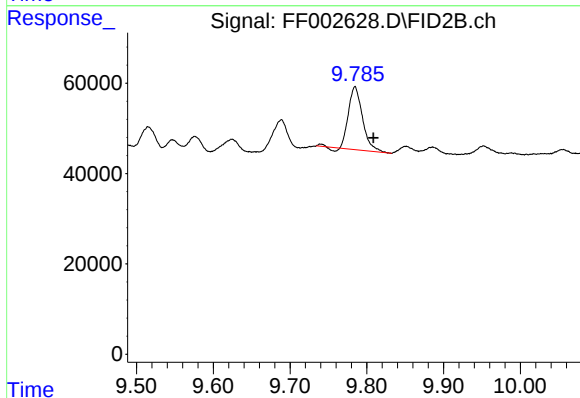


#7 N-HEXADECANE

R.T.: 9.785 min
Delta R.T.: -0.024 min
Response: 175660
Conc: 1.56 ug/ml

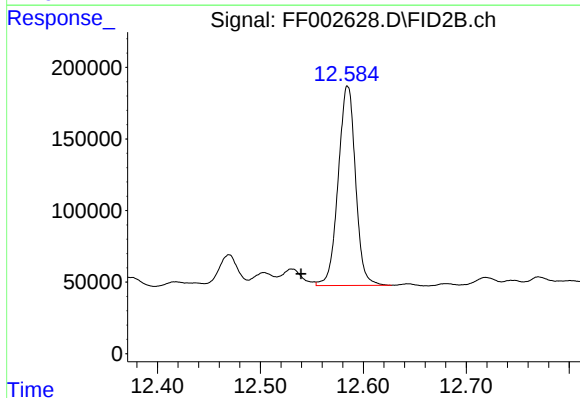


#9 N-EICOSANE

R.T.: 12.585 min
Delta R.T.: 0.045 min
Response: 1630551
Conc: 14.62 ug/ml

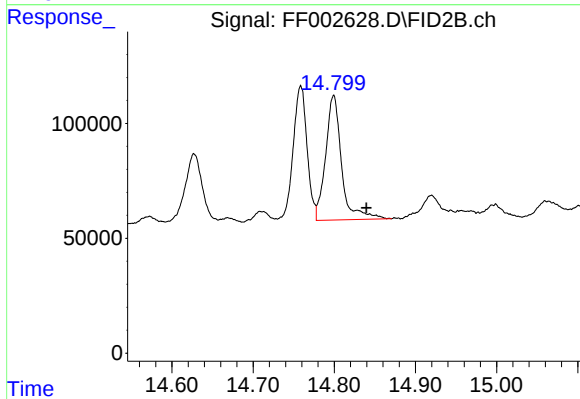


#10 N-TETRACOSANE

R.T.: 14.799 min
Delta R.T.: -0.040 min
Response: 744549
Conc: 6.95 ug/ml

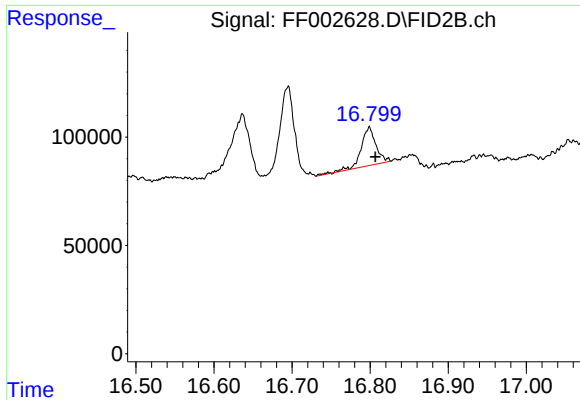


#11 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: -0.008 min
Response: 235708
Conc: 2.26 ug/ml

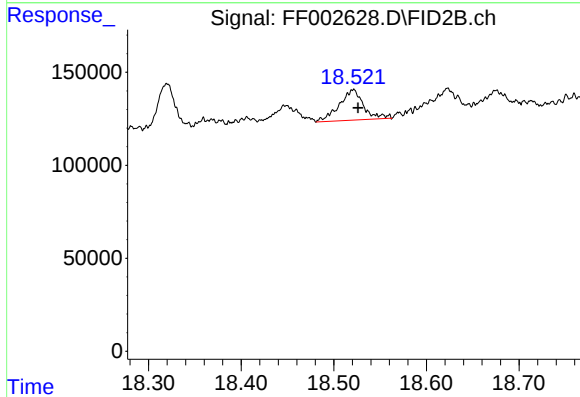

#12 N-DOTRIACONTANE

R.T.: 18.521 min
Delta R.T.: -0.006 min
Response: 299848
Conc: 3.15 ug/ml

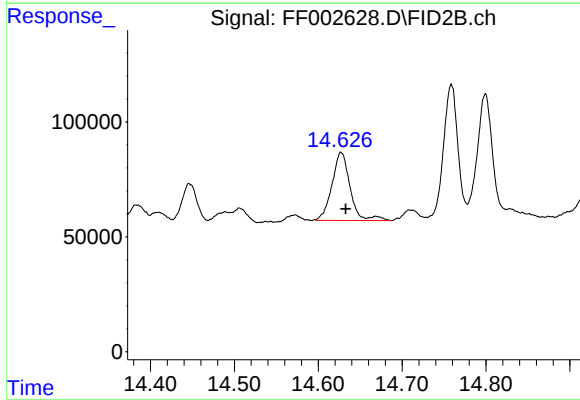

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.006 min
Response: 446275
Conc: 3.56 ug/ml