

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
 Data File : FF005940.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2019 11:12
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Nov 08 23:06:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.414	3455409	26.551 ug/ml
12) N-OCTACOSANE	16.814	3364494	27.205 ug/ml
13) N-TRIACONTANE	17.697	98678	0.813 ug/ml
16) N-HEXATRIACONTANE	20.092	144389	1.437 ug/ml
18) N-TETRACONTANE	21.699	276724	3.091 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
Data File : FF005940.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2019 11:12
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 08 23:06:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

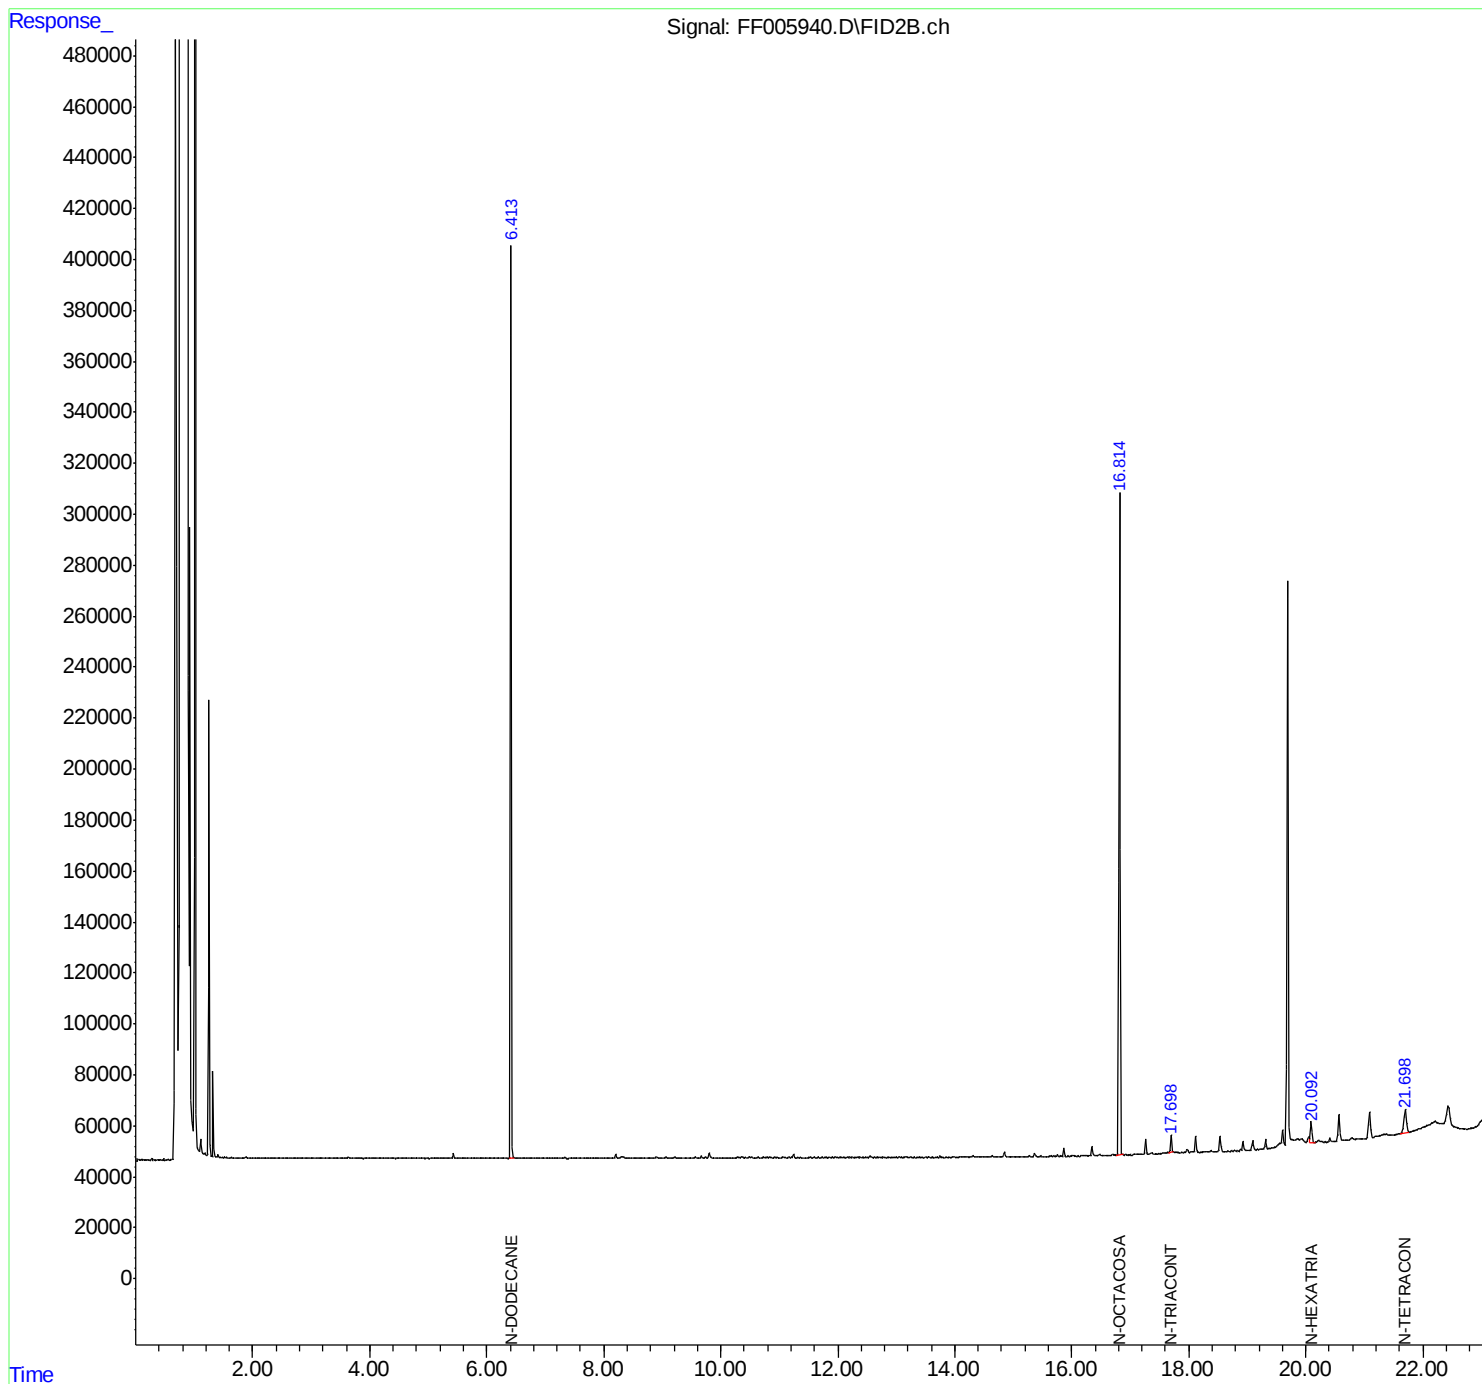


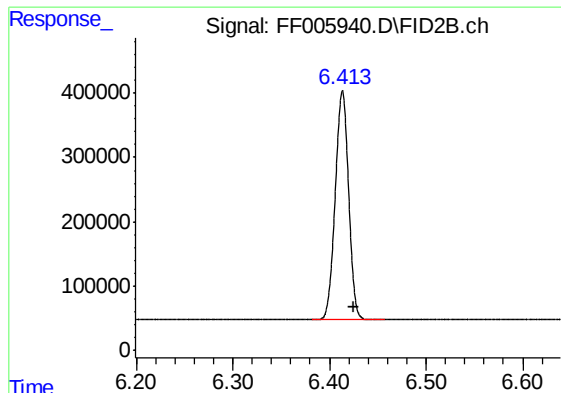

#3 N-DODECANE


R.T.: 6.414 min
Delta R.T.: -0.011 min
Response: 3455409
Conc: 26.55 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

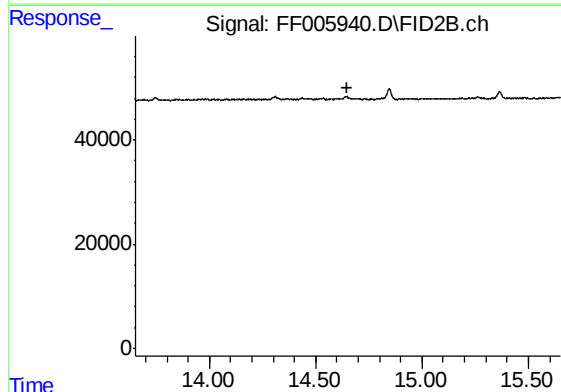


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.651 min
Response: 0
Conc: N.D.

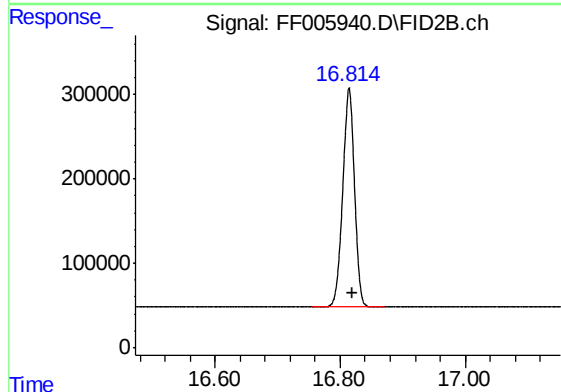


#12 N-OCTACOSANE

R.T.: 16.814 min
Delta R.T.: -0.005 min
Response: 3364494
Conc: 27.20 ug/ml

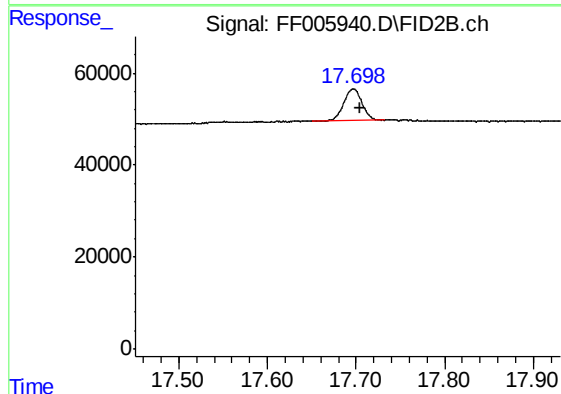

#13 N-TRIACONTANE


R.T.: 17.697 min
Delta R.T.: -0.008 min
Response: 98678
Conc: 0.81 ug/ml

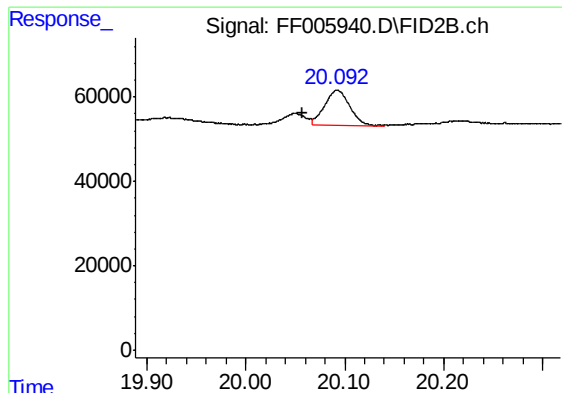

#16 N-HEXATRIACONTANE

R.T.: 20.092 min
Delta R.T.: 0.035 min
Response: 144389
Conc: 1.44 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

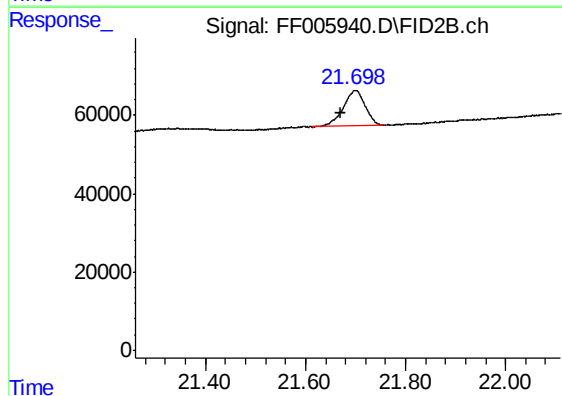

#18 N-TETRACONTANE

R.T.: 21.699 min
Delta R.T.: 0.028 min
Response: 276724
Conc: 3.09 ug/ml