

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
 Data File : FF005941.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2019 13:45
 Operator : DD\AJ
 Sample : K5742-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-38-(2-4)

Integration File: autoint1.e
 Quant Time: Nov 08 23:06:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	1884680	16.769 ug/ml
Target Compounds			
4) N-TETRADECANE	8.260	631688	4.847 ug/ml
8) N-DOCOSANE	13.743	113207	0.874 ug/ml
12) N-OCTACOSANE	16.810	117654	0.951 ug/ml
13) N-TRIACONTANE	17.696	204116	1.682 ug/ml
14) N-DOTRIACONTANE	18.528	161826	1.414 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
Data File : FF005941.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2019 13:45
Operator : DD\AJ
Sample : K5742-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)

Integration File: autoint1.e
Quant Time: Nov 08 23:06:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

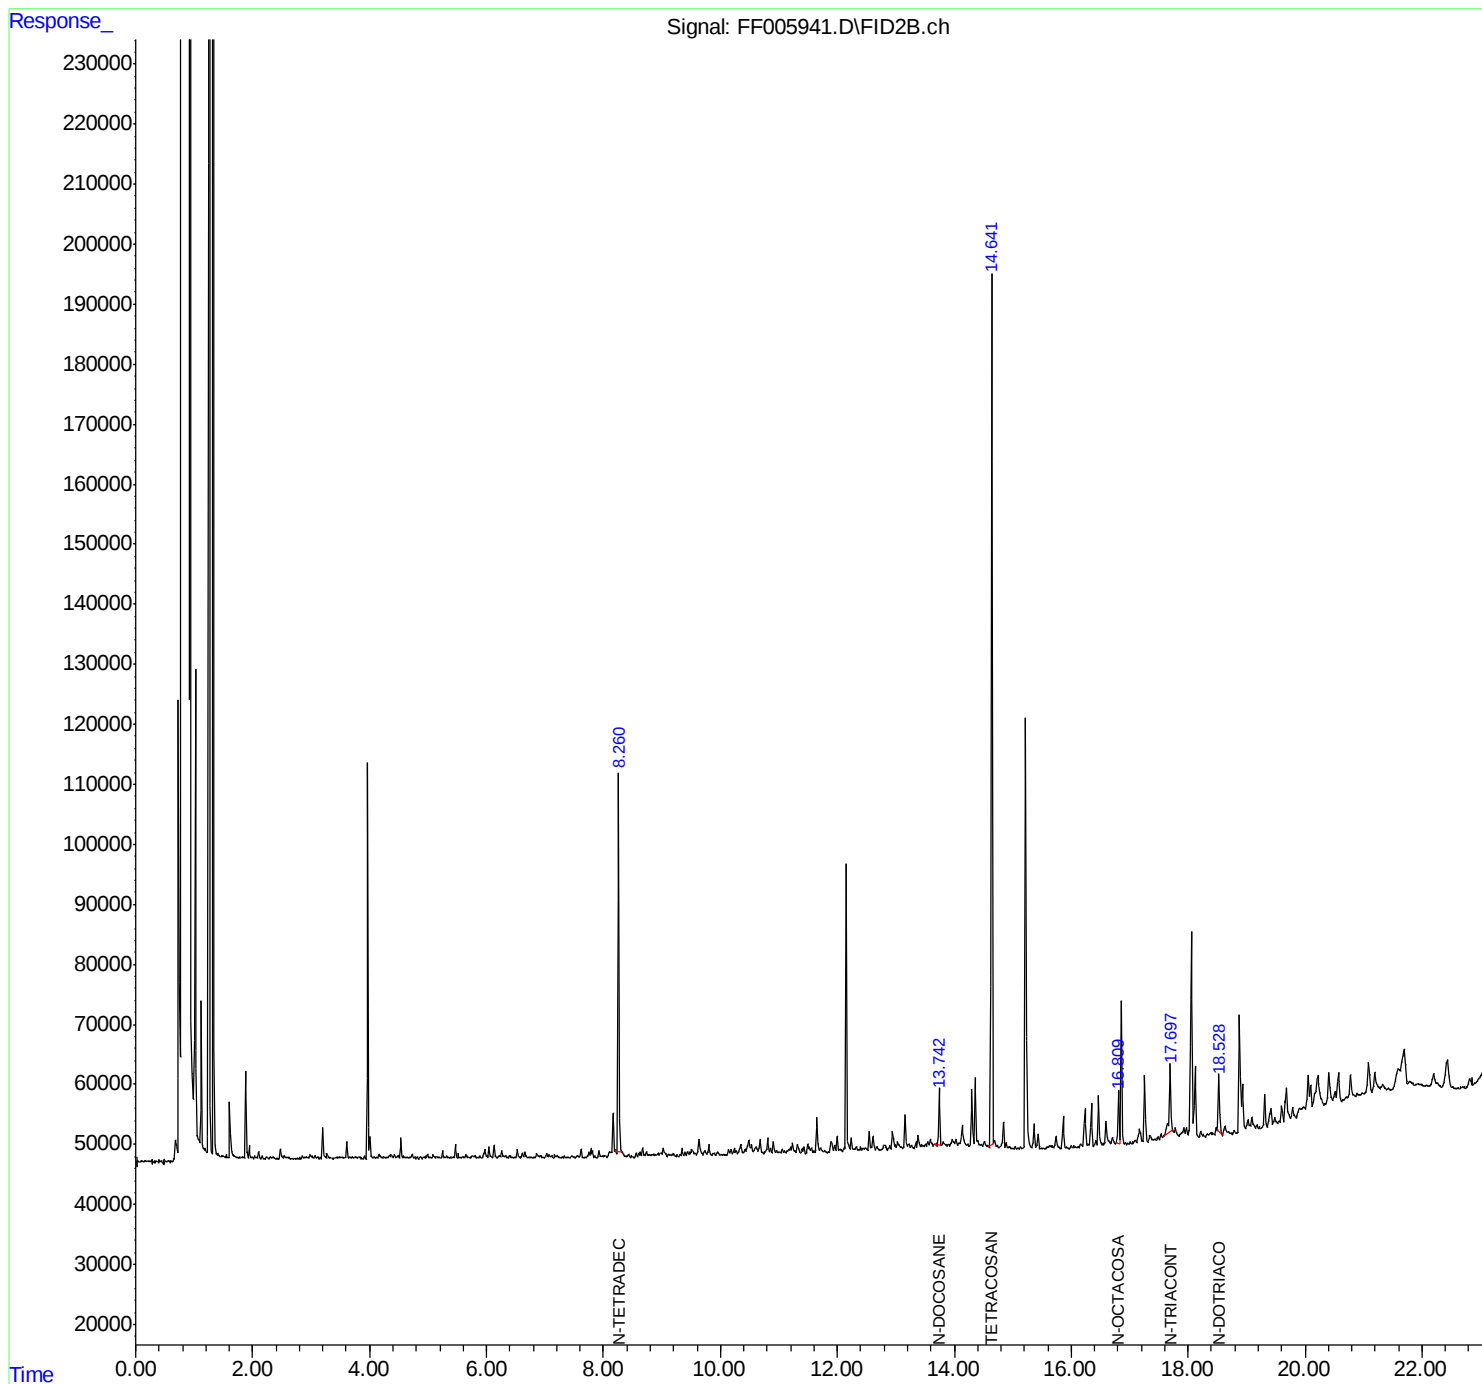


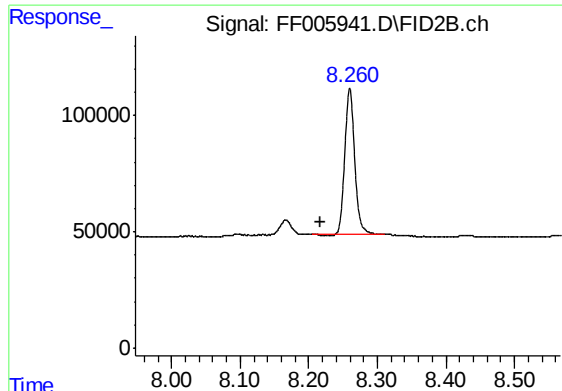

#4 N-TETRADECANE


R.T.: 8.260 min
Delta R.T.: 0.044 min
Response: 631688
Conc: 4.85 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)

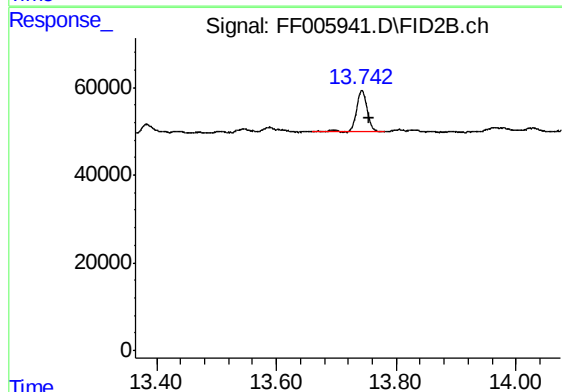


#8 N-DOCOSANE

R.T.: 13.743 min
Delta R.T.: -0.012 min
Response: 113207
Conc: 0.87 ug/ml

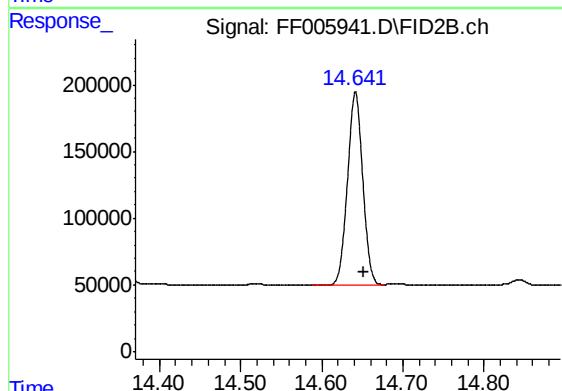


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: -0.010 min
Response: 1884680
Conc: 16.77 ug/ml

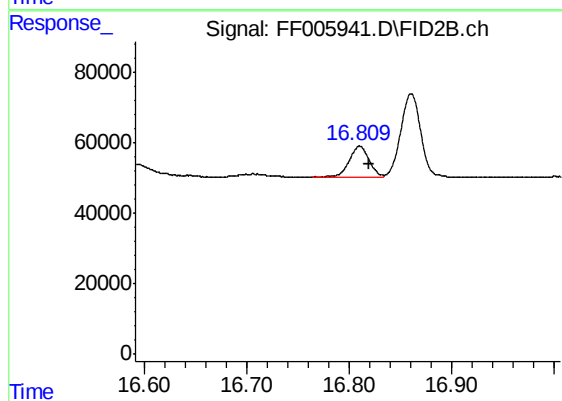

#12 N-OCTACOSANE


R.T.: 16.810 min
Delta R.T.: -0.009 min
Response: 117654
Conc: 0.95 ug/ml

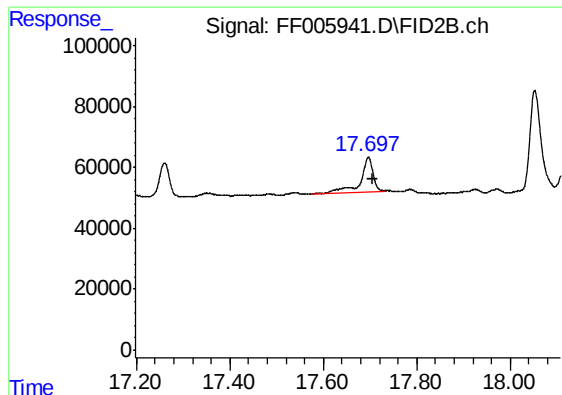

#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: -0.009 min
Response: 204116
Conc: 1.68 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)

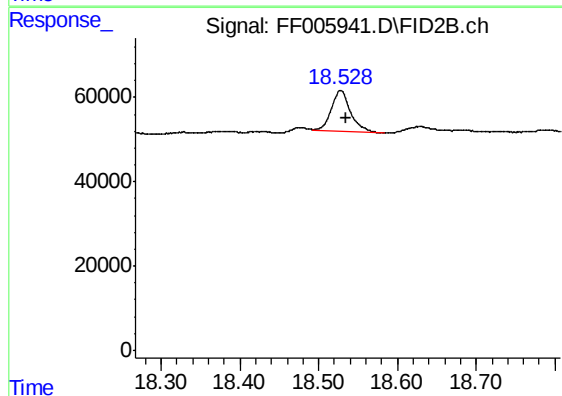

#14 N-DOTRIACONTANE

R.T.: 18.528 min
Delta R.T.: -0.007 min
Response: 161826
Conc: 1.41 ug/ml