

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
Data File : FF005946.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2019 16:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 08 23:07:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.644	2387390	21.242 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.696	56446	0.465 ug/ml
16)	N-HEXATRIACONTANE	20.094	368170	3.665 ug/ml
18)	N-TETRACONTANE	21.701	346366	3.869 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
Data File : FF005946.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2019 16:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 08 23:07:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

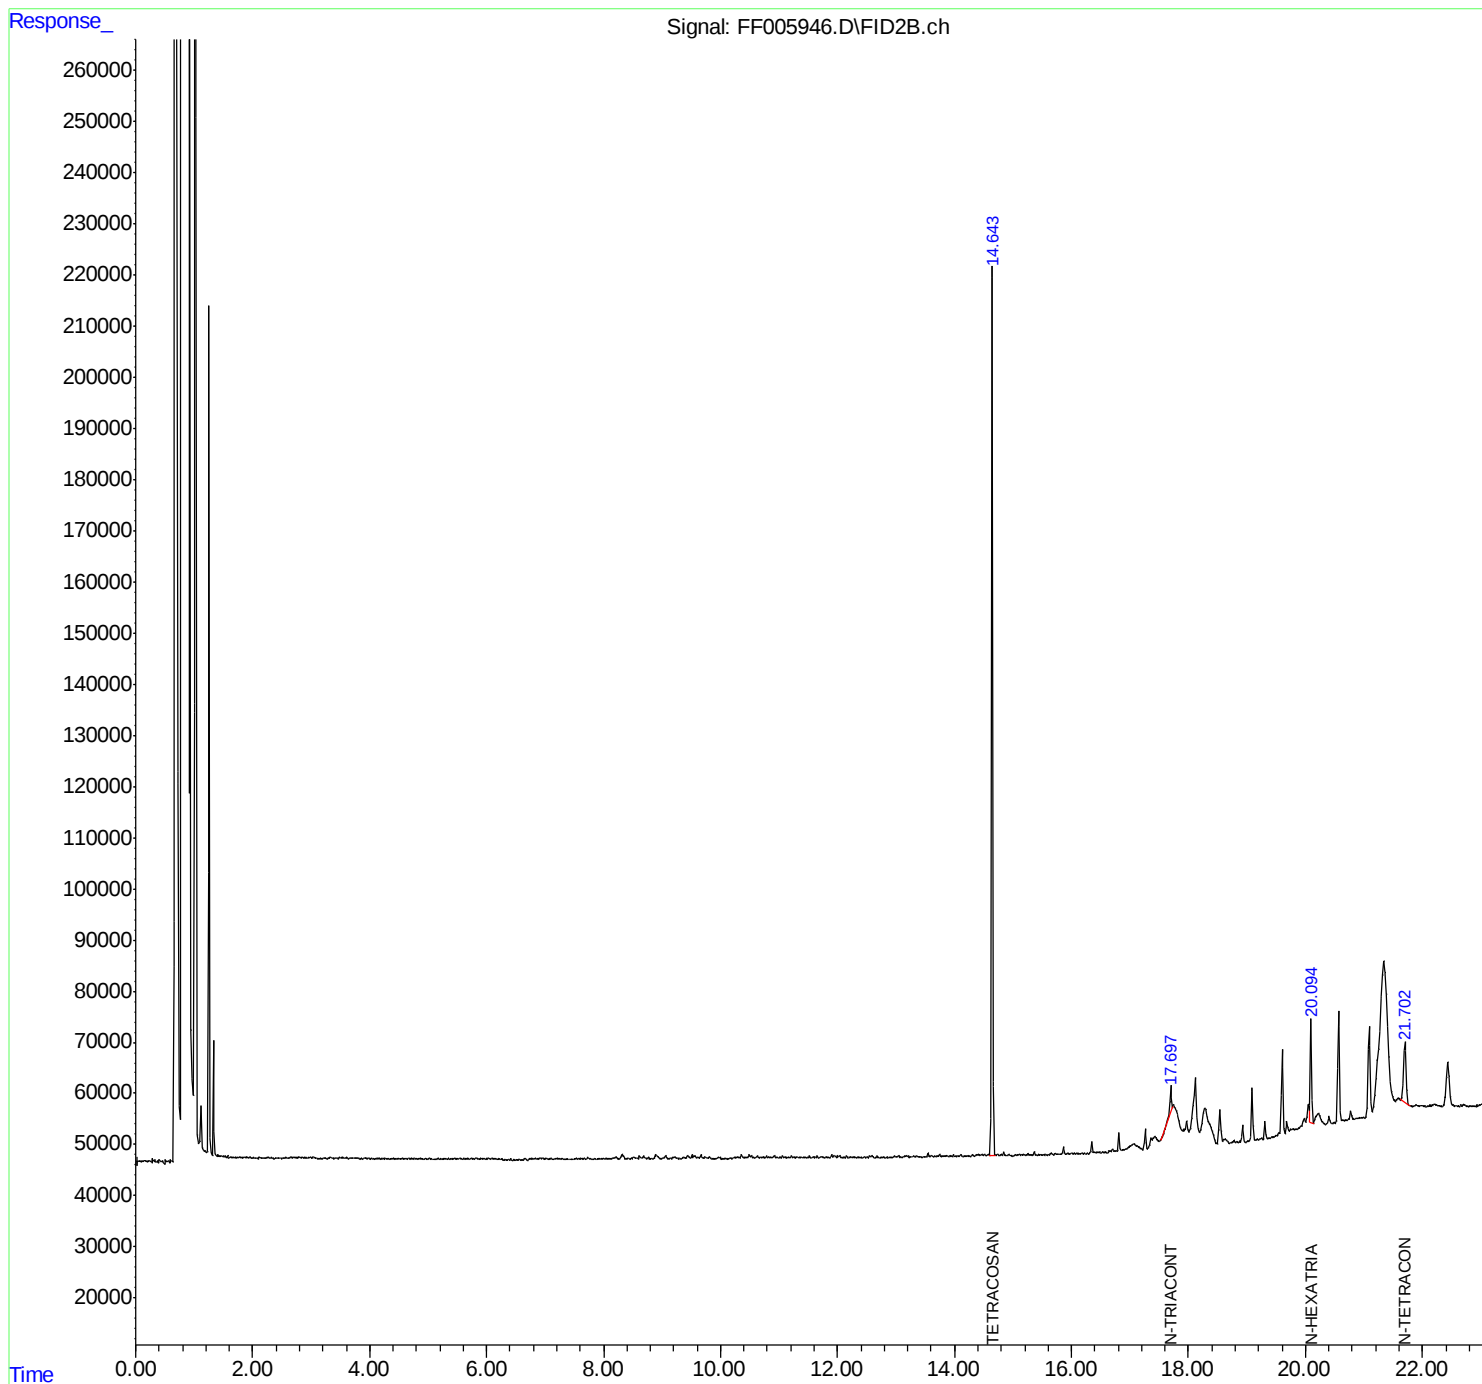


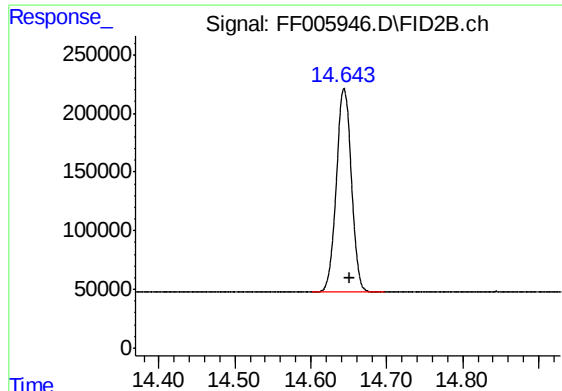

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.644 min
Delta R.T.: -0.008 min
Response: 2387390
Conc: 21.24 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

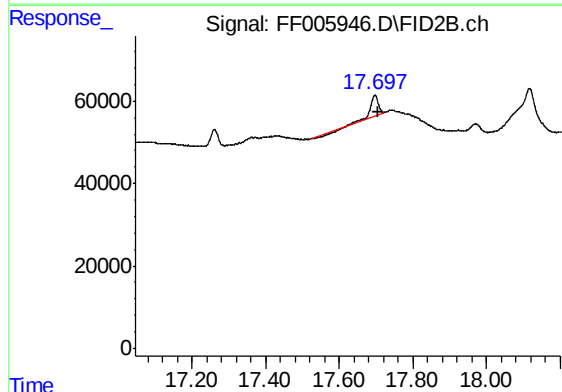


#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: -0.009 min
Response: 56446
Conc: 0.47 ug/ml

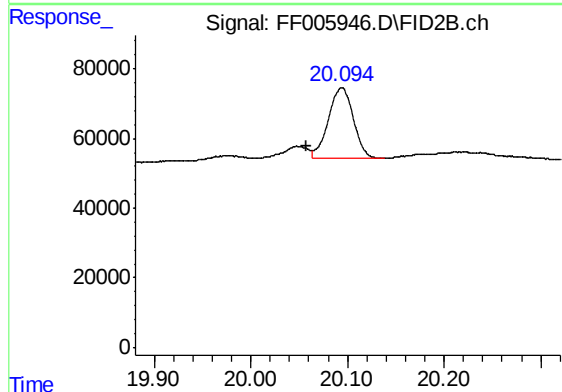

#16 N-HEXATRIACONTANE

R.T.: 20.094 min
Delta R.T.: 0.037 min
Response: 368170
Conc: 3.67 ug/ml

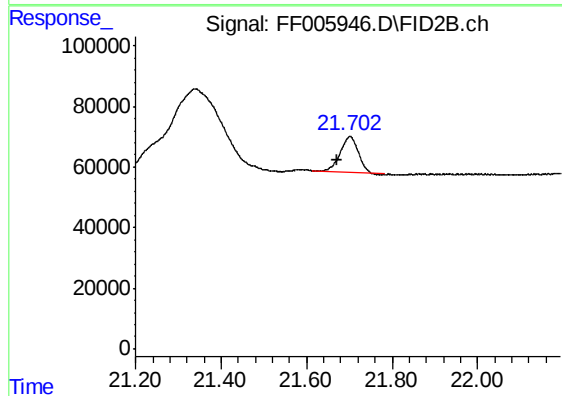

#18 N-TETRACONTANE

R.T.: 21.701 min
Delta R.T.: 0.030 min
Response: 346366
Conc: 3.87 ug/ml