

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
 Data File : FF005939.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2019 10:20
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Nov 08 23:06:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	6063936	53.955 ug/ml
Target Compounds			
2) N-DECANE	4.407	7059504	54.968 ug/ml
3) N-DODECANE	6.424	7184809	55.207 ug/ml
4) N-TETRADECANE	8.215	7170753	55.019 ug/ml
5) N-HEXADECANE	9.812	7197933	54.658 ug/ml
6) N-OCTADECANE	11.250	7084293	54.324 ug/ml
7) N-EICOSANE	12.557	7085797	54.046 ug/ml
8) N-DOCOSANE	13.751	6967646	53.788 ug/ml
10) N-TETRACOSANE	14.852	6859847	53.561 ug/ml
11) N-HEXACOSANE	15.869	6724367	53.291 ug/ml
12) N-OCTACOSANE	16.817	6562967	53.067 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
Data File : FF005939.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2019 10:20
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Nov 08 23:06:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

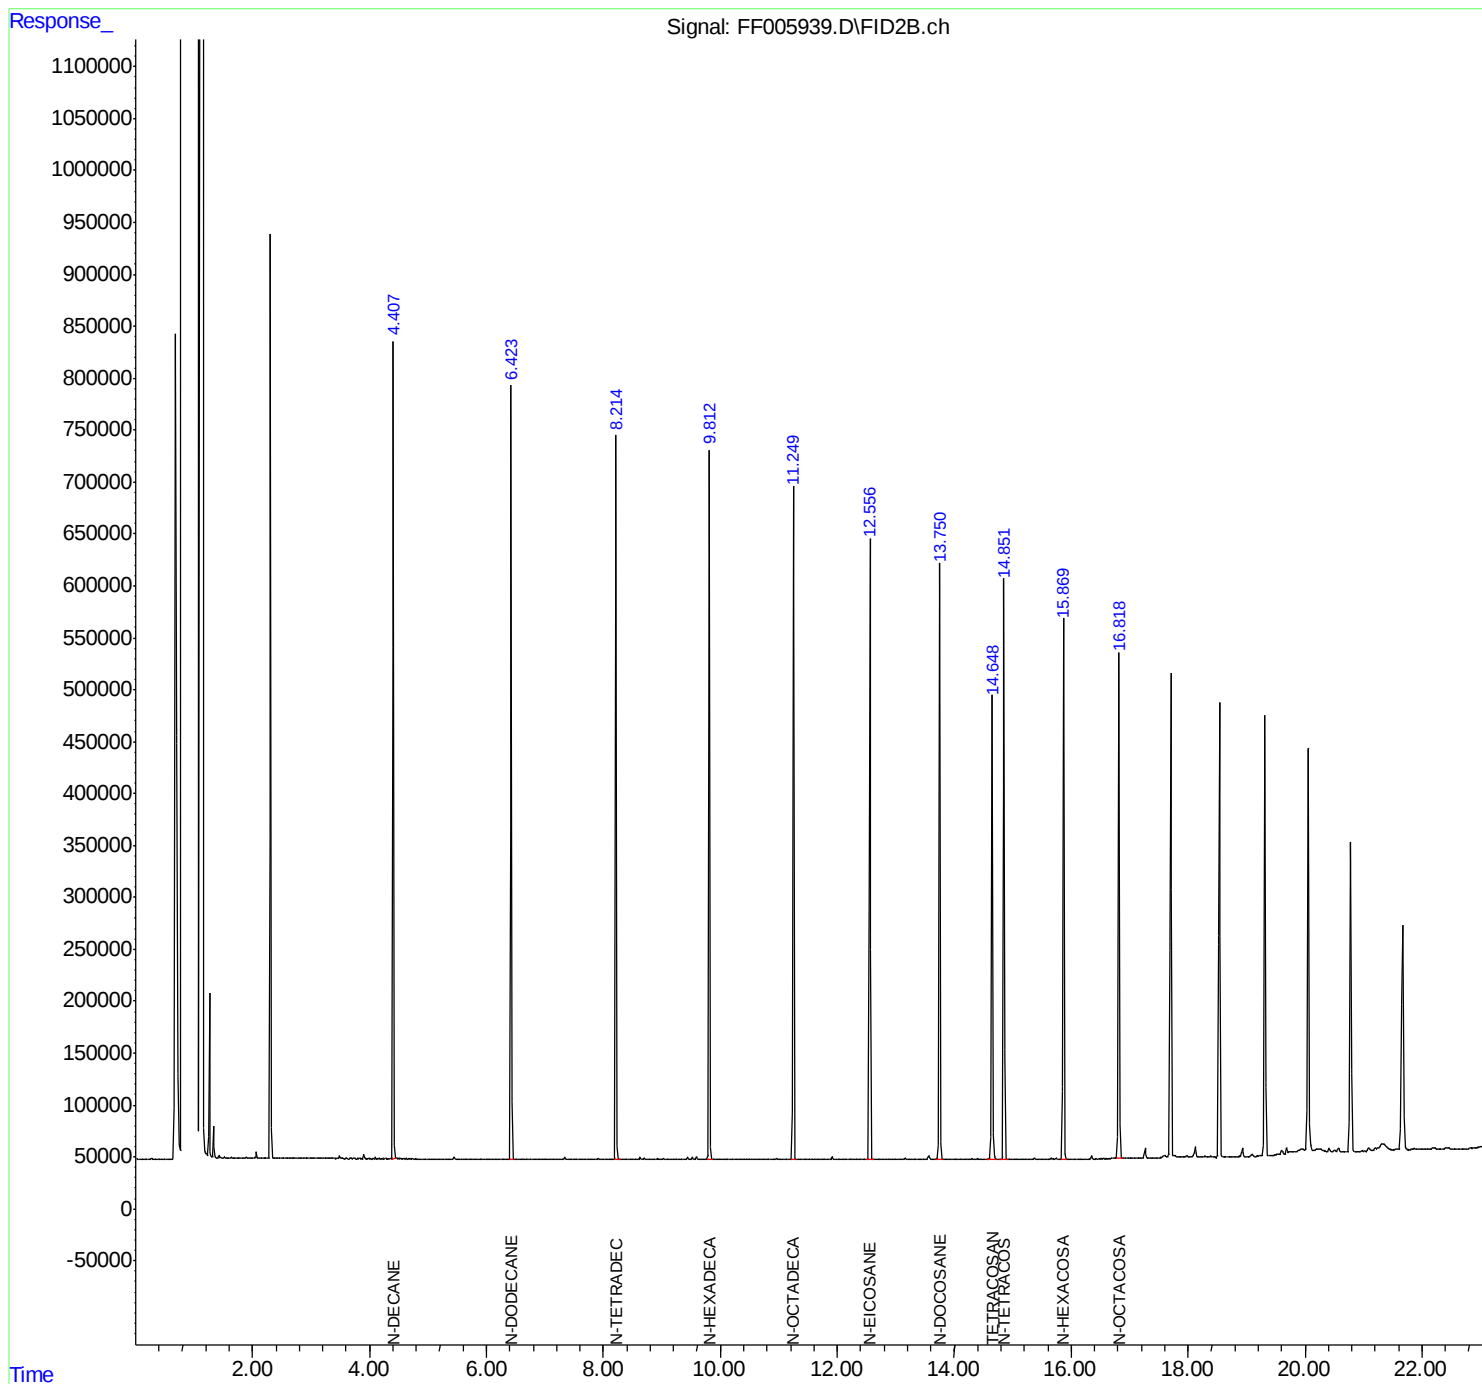


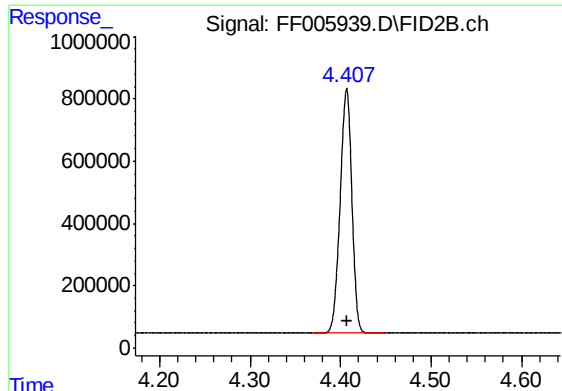

#2 N-DECANE


R.T.: 4.407 min
Delta R.T.: 0.000 min
Response: 7059504
Conc: 54.97 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

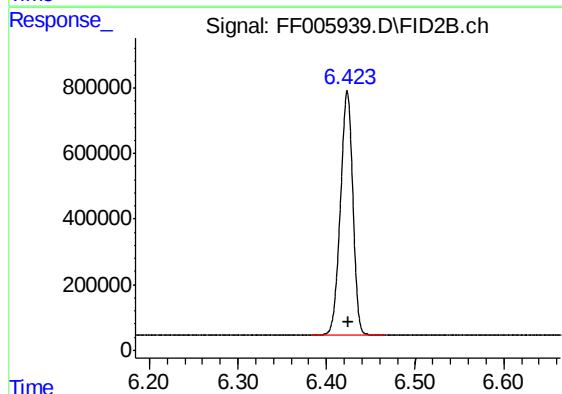


#3 N-DODECANE

R.T.: 6.424 min
Delta R.T.: -0.001 min
Response: 7184809
Conc: 55.21 ug/ml

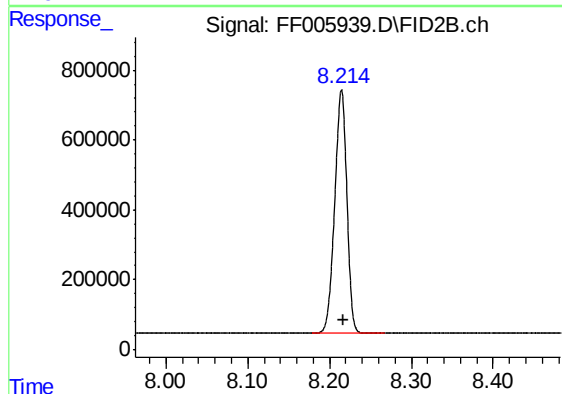


#4 N-TETRADECANE

R.T.: 8.215 min
Delta R.T.: -0.002 min
Response: 7170753
Conc: 55.02 ug/ml

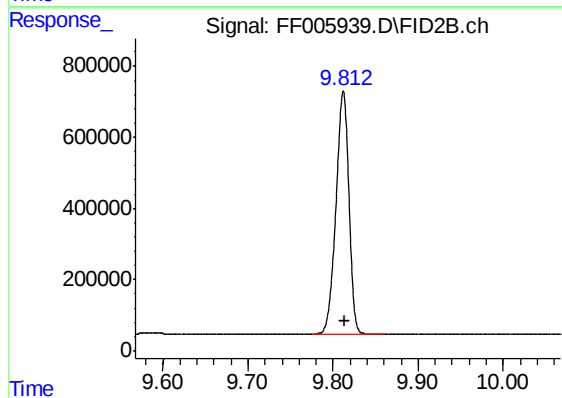

#5 N-HEXADECANE


R.T.: 9.812 min
Delta R.T.: -0.002 min
Response: 7197933
Conc: 54.66 ug/ml

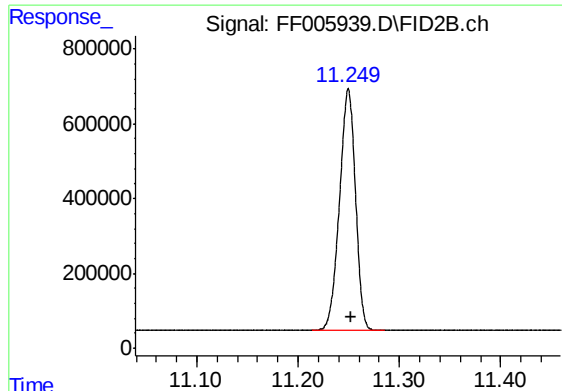

#6 N-OCTADECANE


R.T.: 11.250 min
Delta R.T.: -0.003 min
Response: 7084293
Conc: 54.32 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

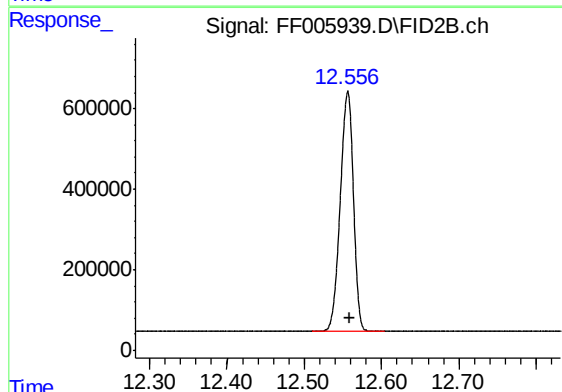


#7 N-EICOSANE

R.T.: 12.557 min
Delta R.T.: -0.002 min
Response: 7085797
Conc: 54.05 ug/ml

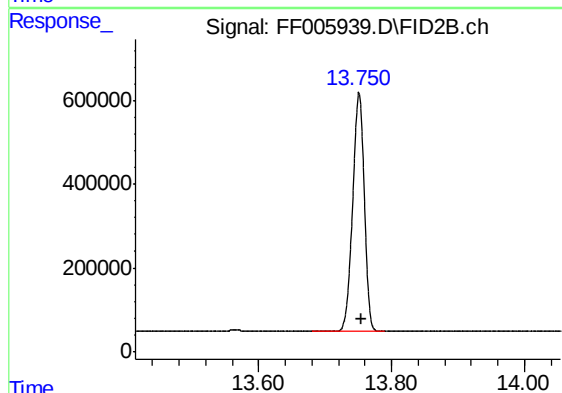


#8 N-DOCOSANE

R.T.: 13.751 min
Delta R.T.: -0.004 min
Response: 6967646
Conc: 53.79 ug/ml

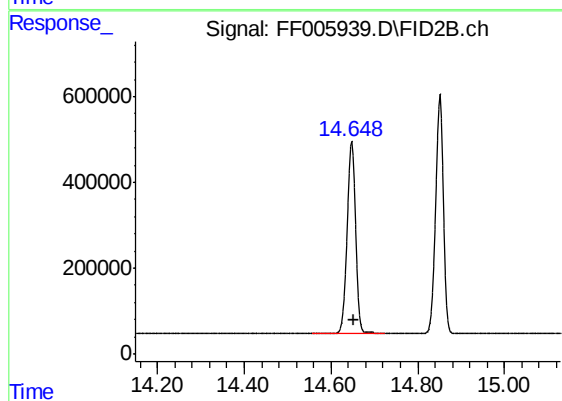

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.648 min
Delta R.T.: -0.004 min
Response: 6063936
Conc: 53.96 ug/ml

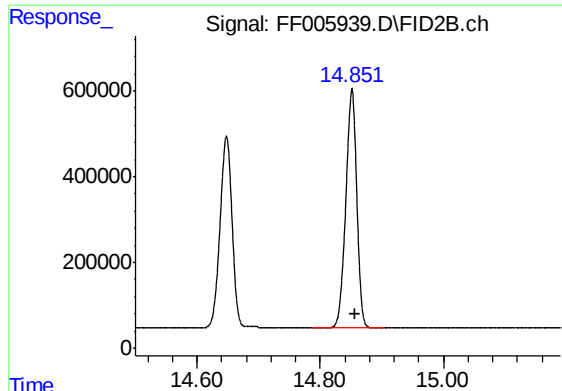

#10 N-TETRACOSANE


R.T.: 14.852 min
Delta R.T.: -0.004 min
Response: 6859847
Conc: 53.56 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

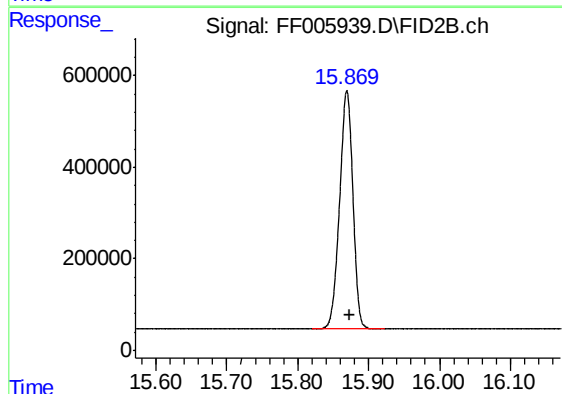

#11 N-HEXACOSANE

R.T.: 15.869 min
Delta R.T.: -0.003 min
Response: 6724367
Conc: 53.29 ug/ml

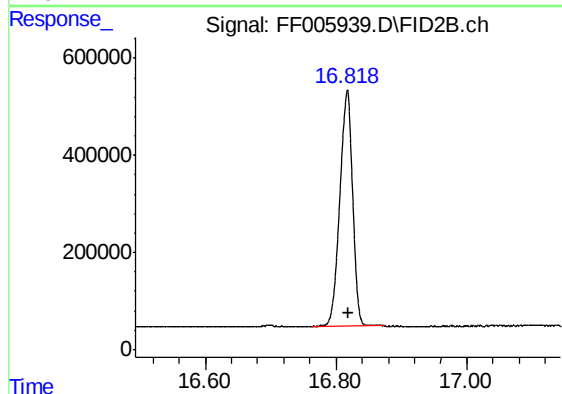

#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.002 min
Response: 6562967
Conc: 53.07 ug/ml