

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
 Data File : FF005942.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2019 14:14
 Operator : DD\AJ
 Sample : K5742-11MS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-38-(2-4)MS

Integration File: autoint1.e
 Quant Time: Nov 08 23:06:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
 Quant Title :
 QLast Update : Wed Nov 06 11:58:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.645	2392768	21.290 ug/ml
Target Compounds			
2) N-DECANE	4.404	2813872	21.910 ug/ml
3) N-DODECANE	6.419	2896428	22.256 ug/ml
4) N-TETRADECANE	8.210	2934435	22.515 ug/ml
5) N-HEXADECANE	9.806	2984668	22.664 ug/ml
6) N-OCTADECANE	11.245	2981130	22.860 ug/ml
7) N-EICOSANE	12.552	2974384	22.687 ug/ml
8) N-DOCOSANE	13.748	3035478	23.433 ug/ml
10) N-TETRACOSANE	14.848	2924055	22.831 ug/ml
11) N-HEXACOSANE	15.867	2885248	22.866 ug/ml
12) N-OCTACOSANE	16.814	2918712	23.600 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110819\
Data File : FF005942.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2019 14:14
Operator : DD\AJ
Sample : K5742-11MS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)MS

Integration File: autoint1.e
Quant Time: Nov 08 23:06:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

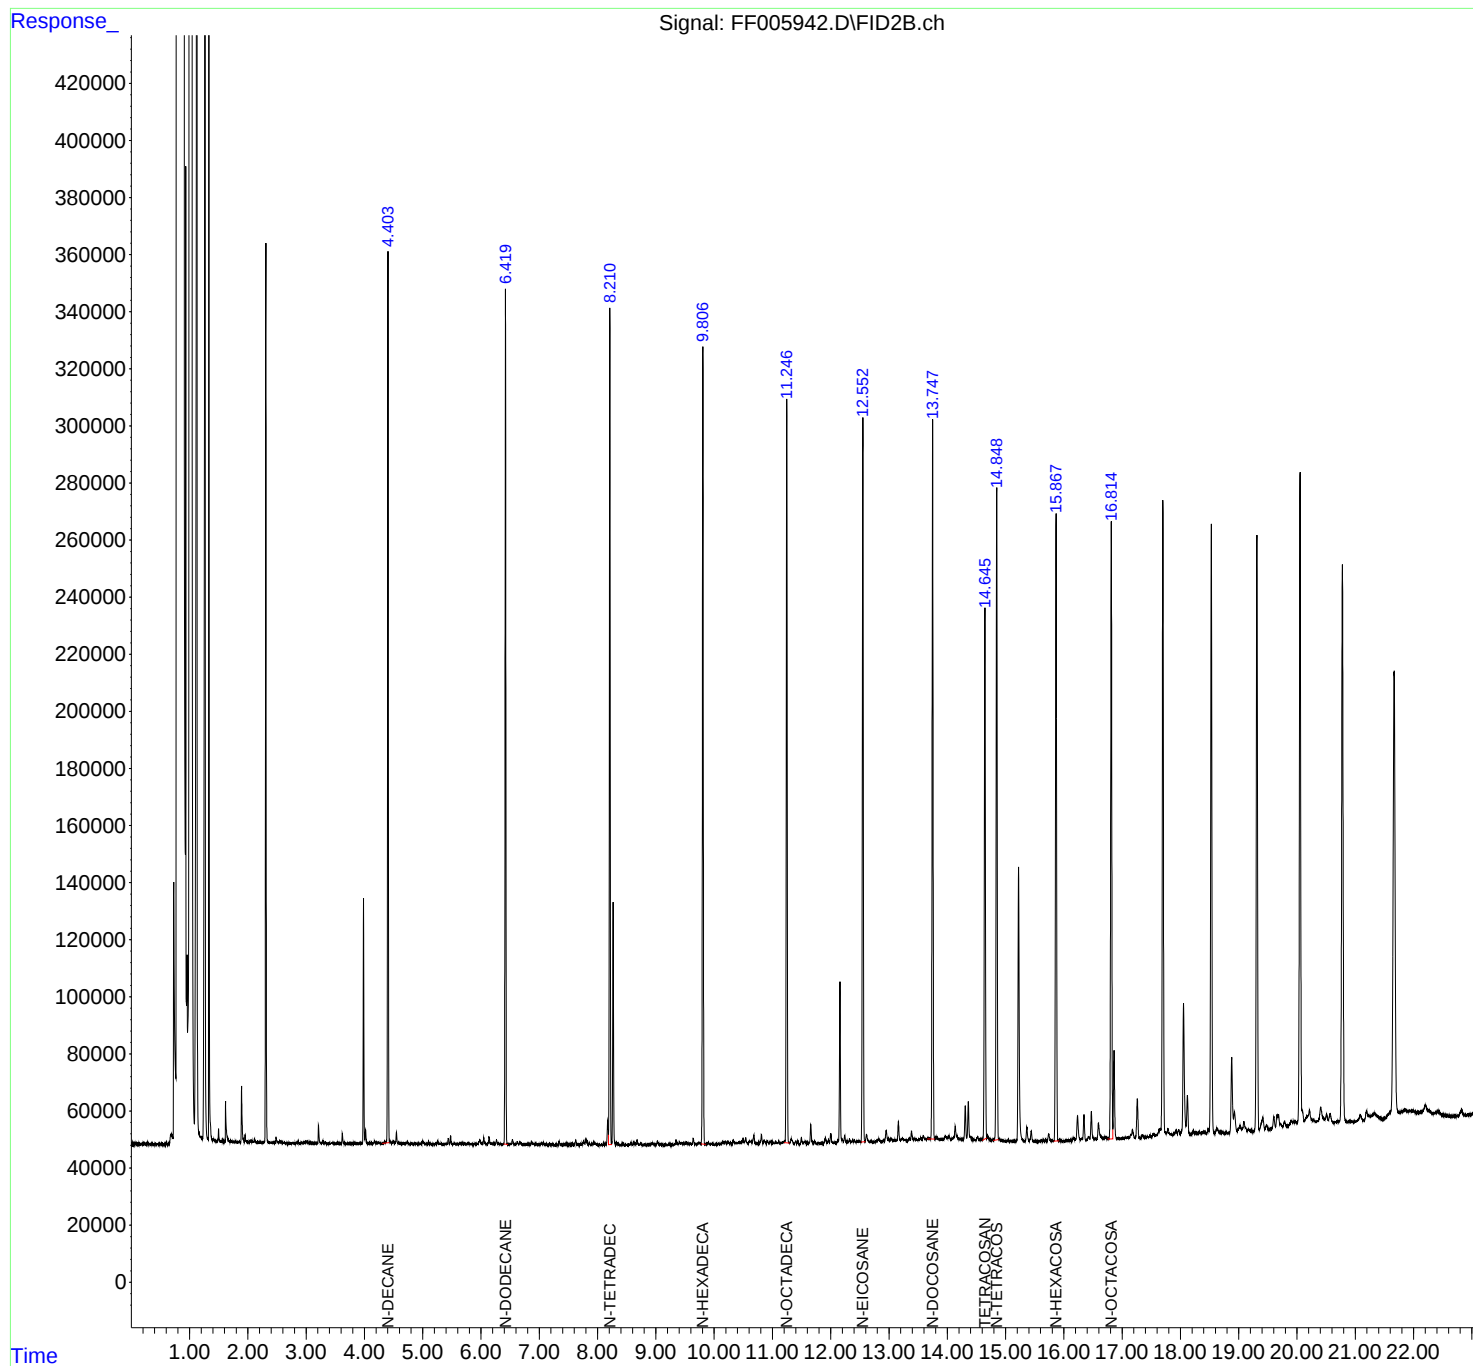


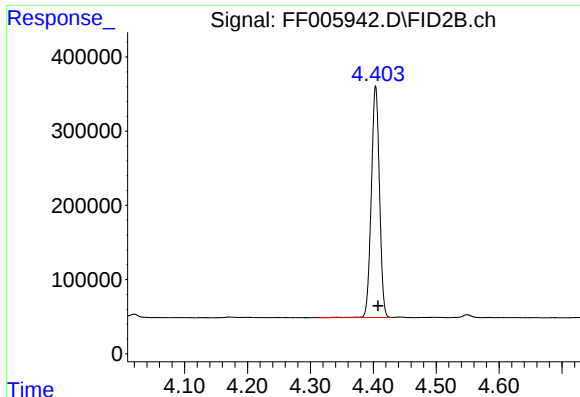

#2 N-DECANE


R.T.: 4.404 min
Delta R.T.: -0.004 min
Response: 2813872
Conc: 21.91 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)MS

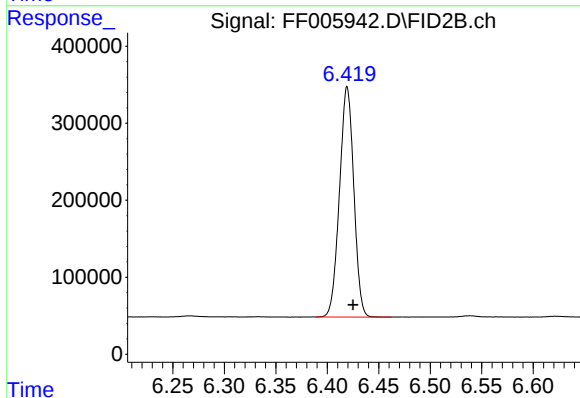


#3 N-DODECANE

R.T.: 6.419 min
Delta R.T.: -0.006 min
Response: 2896428
Conc: 22.26 ug/ml

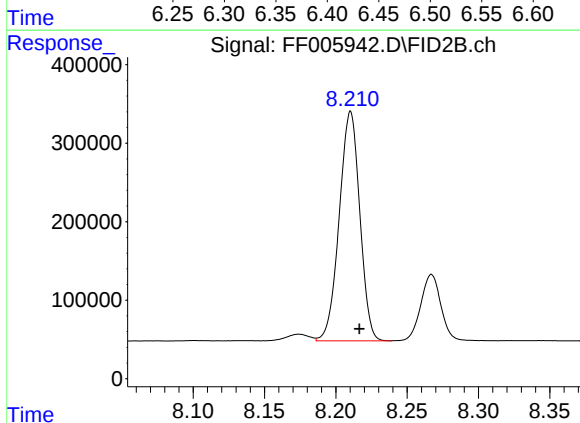


#4 N-TETRADECANE

R.T.: 8.210 min
Delta R.T.: -0.006 min
Response: 2934435
Conc: 22.51 ug/ml

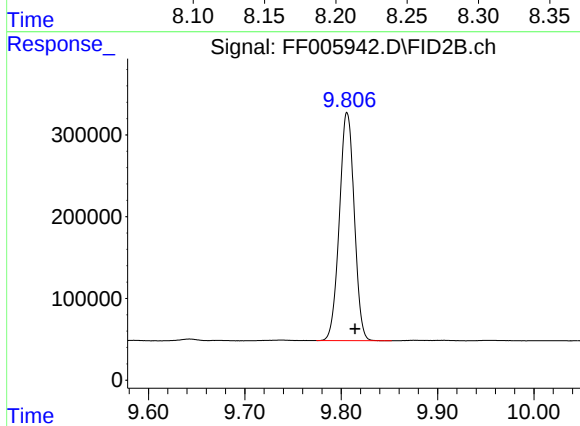

#5 N-HEXADECANE


R.T.: 9.806 min
Delta R.T.: -0.008 min
Response: 2984668
Conc: 22.66 ug/ml

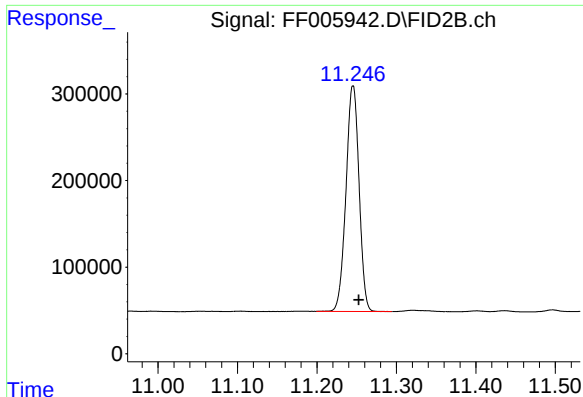

#6 N-OCTADECANE


R.T.: 11.245 min
Delta R.T.: -0.007 min
Response: 2981130
Conc: 22.86 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)MS

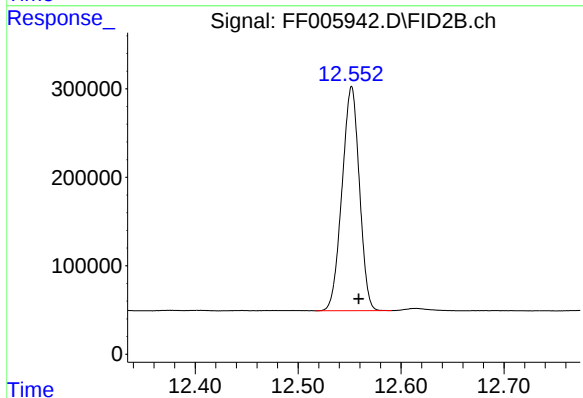


#7 N-EICOSANE

R.T.: 12.552 min
Delta R.T.: -0.007 min
Response: 2974384
Conc: 22.69 ug/ml

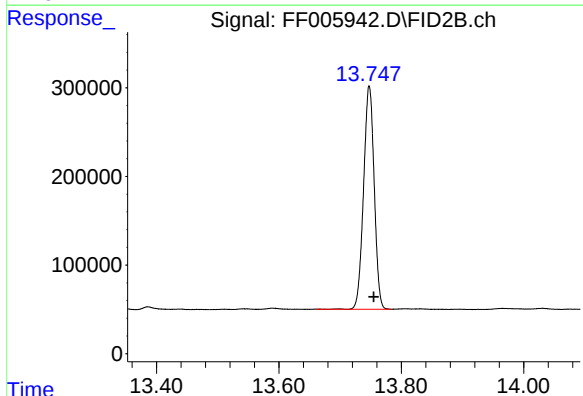


#8 N-DOCOSANE

R.T.: 13.748 min
Delta R.T.: -0.007 min
Response: 3035478
Conc: 23.43 ug/ml

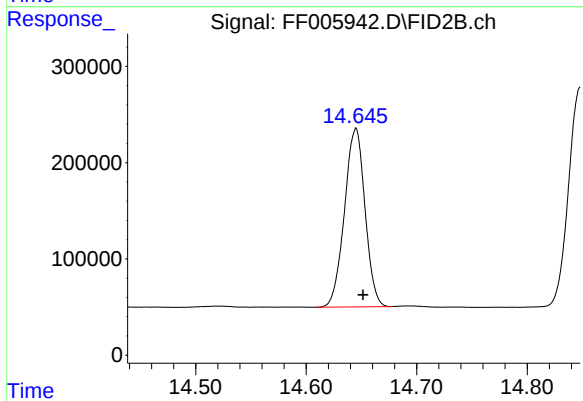

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.645 min
Delta R.T.: -0.006 min
Response: 2392768
Conc: 21.29 ug/ml

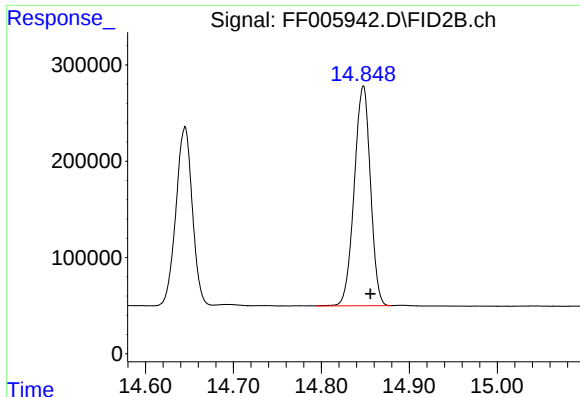

#10 N-TETRACOSANE


R.T.: 14.848 min
Delta R.T.: -0.008 min
Response: 2924055
Conc: 22.83 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-38-(2-4)MS

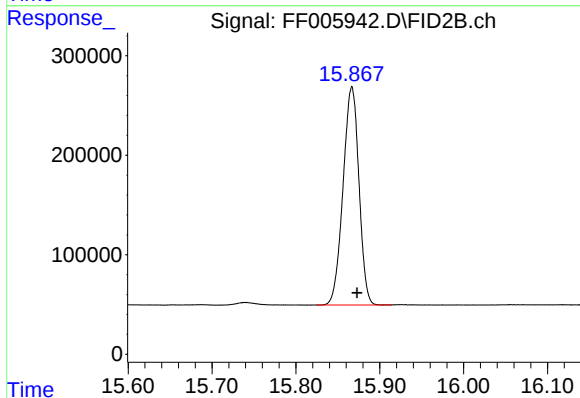

#11 N-HEXACOSANE

R.T.: 15.867 min
Delta R.T.: -0.006 min
Response: 2885248
Conc: 22.87 ug/ml

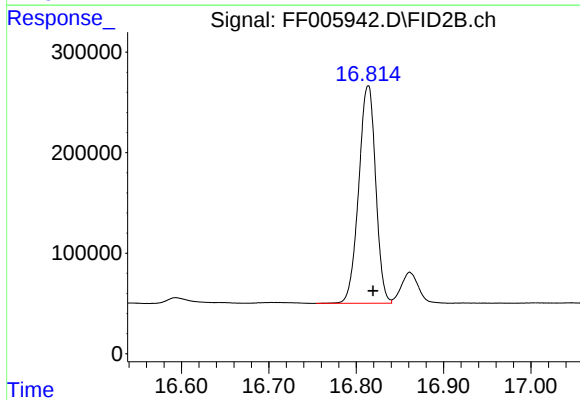

#12 N-OCTACOSANE

R.T.: 16.814 min
Delta R.T.: -0.005 min
Response: 2918712
Conc: 23.60 ug/ml