

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110822\
 Data File : FF011562.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2022 20:10
 Operator : YP\AJ
 Sample : N5494-06MS
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-17MS

Integration File: autoint1.e
 Quant Time: Nov 09 04:59:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.047	1391622	11.729 ug/ml
Target Compounds			
2) N-DECANE	4.613	2016087	15.275 ug/ml
3) N-DODECANE	6.773	2104451	15.658 ug/ml
4) N-TETRADECANE	8.597	2190607	16.187 ug/ml
5) N-HEXADECANE	10.202	2294781	16.692 ug/ml
6) N-OCTADECANE	11.643	2321989	16.786 ug/ml
7) N-EICOSANE	12.951	2265187	16.379 ug/ml
8) N-DOCOSANE	14.149	2242990	16.618 ug/ml
10) N-TETRACOSANE	15.250	2294238	16.918 ug/ml
11) N-HEXACOSANE	16.271	2230135	16.692 ug/ml
12) N-OCTACOSANE	17.221	2160925	16.311 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110822\
Data File : FF011562.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2022 20:10
Operator : YP\AJ
Sample : N5494-06MS
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-17MS

Integration File: autoint1.e
Quant Time: Nov 09 04:59:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

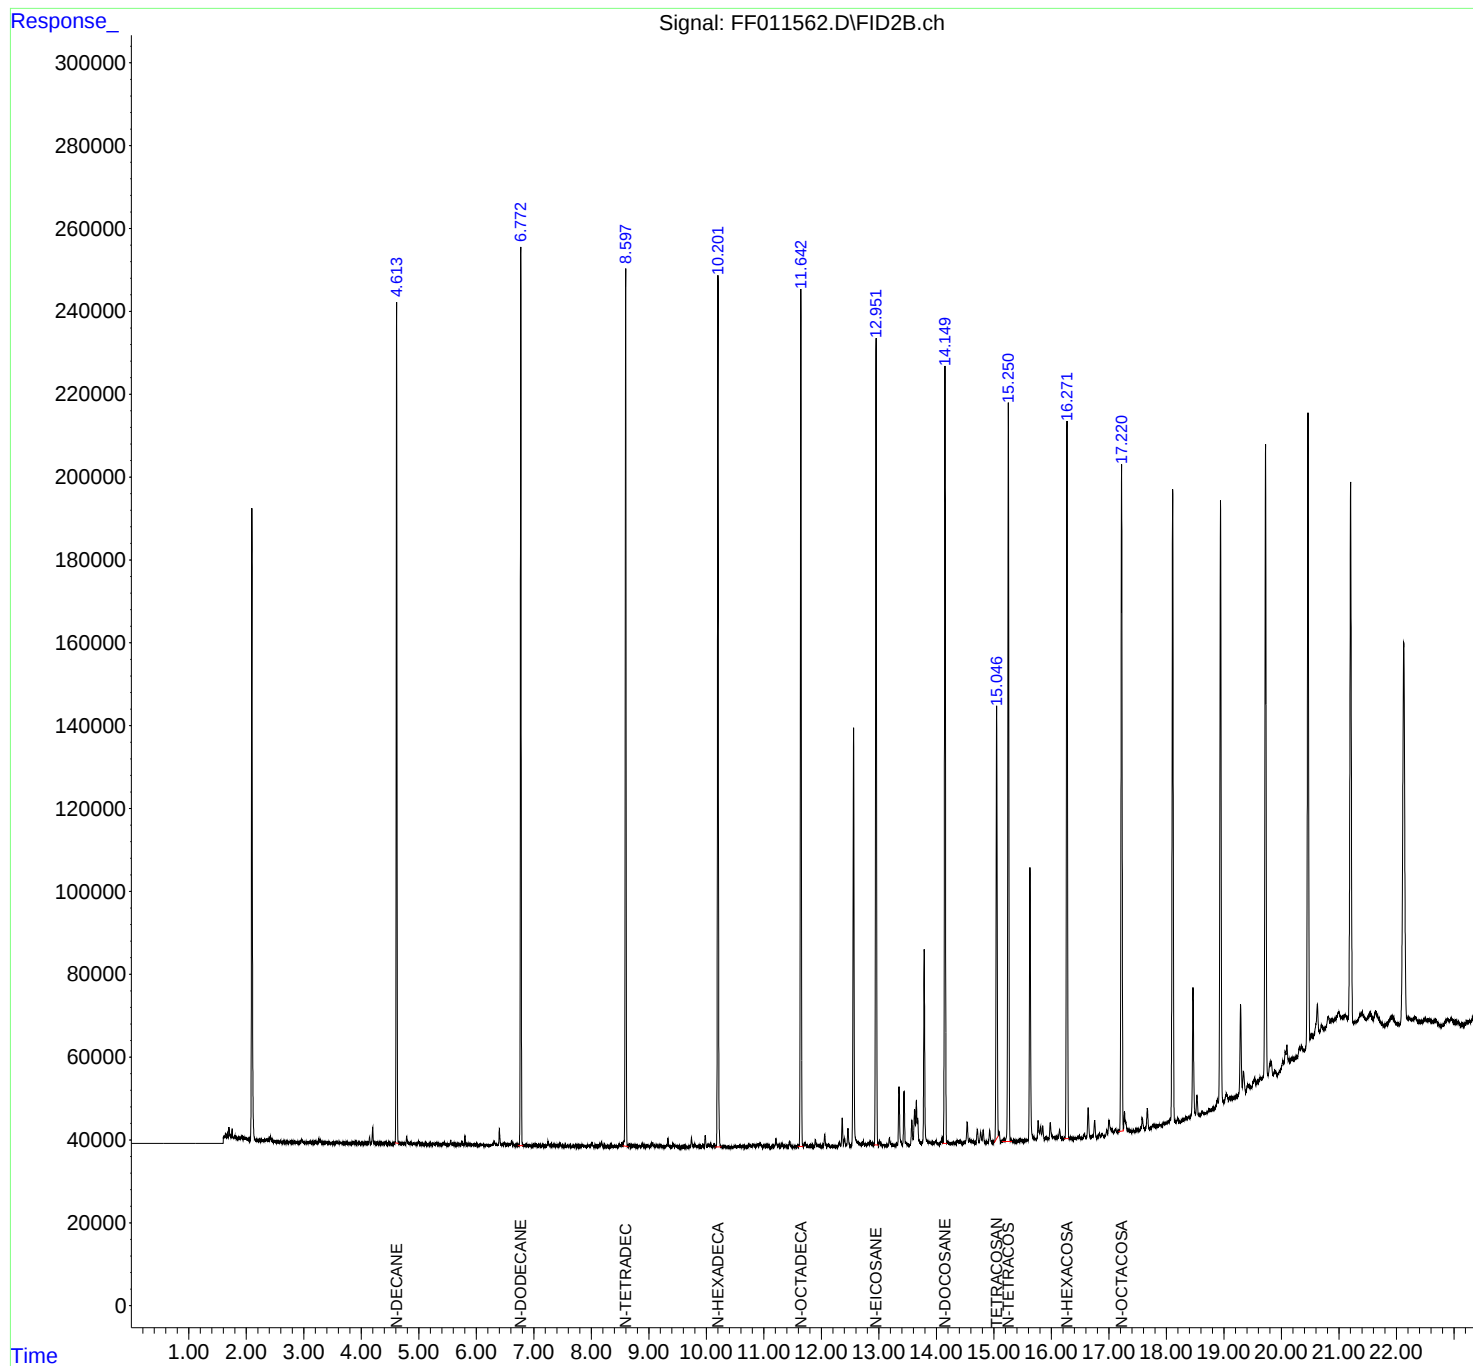


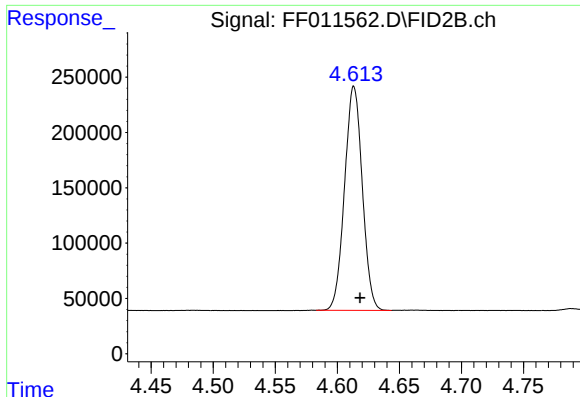

#2 N-DECANE


R.T.: 4.613 min
Delta R.T.: -0.005 min
Response: 2016087
Conc: 15.28 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MS

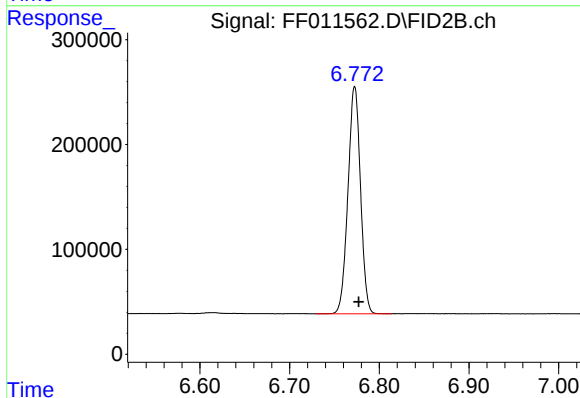


#3 N-DODECANE

R.T.: 6.773 min
Delta R.T.: -0.005 min
Response: 2104451
Conc: 15.66 ug/ml

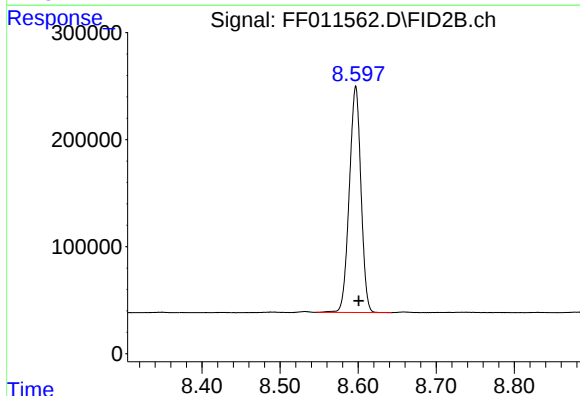


#4 N-TETRADECANE

R.T.: 8.597 min
Delta R.T.: -0.004 min
Response: 2190607
Conc: 16.19 ug/ml

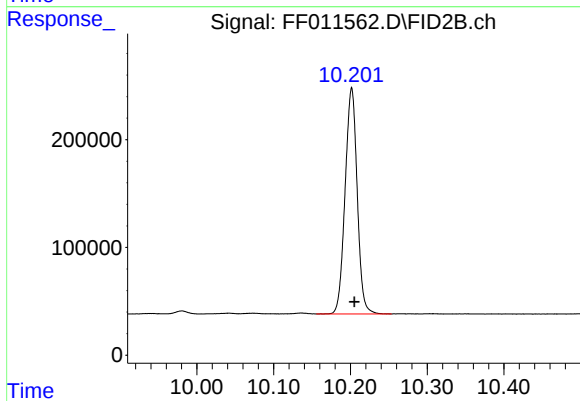

#5 N-HEXADECANE


R.T.: 10.202 min
Delta R.T.: -0.003 min
Response: 2294781
Conc: 16.69 ug/ml

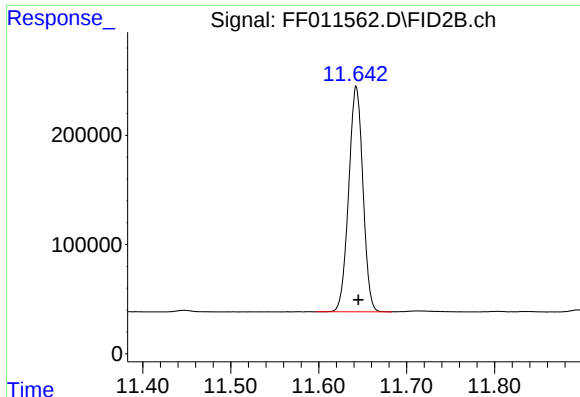

#6 N-OCTADECANE


R.T.: 11.643 min
Delta R.T.: -0.003 min
Response: 2321989
Conc: 16.79 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MS

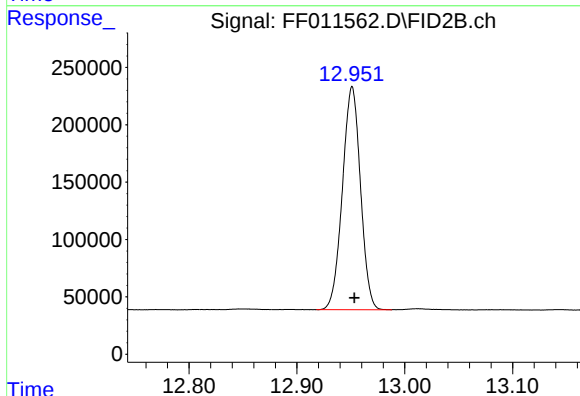


#7 N-EICOSANE

R.T.: 12.951 min
Delta R.T.: -0.002 min
Response: 2265187
Conc: 16.38 ug/ml

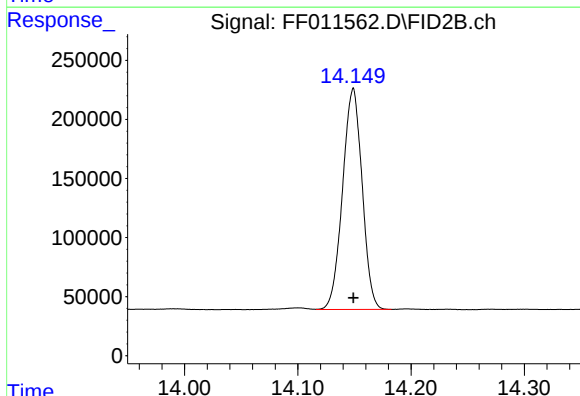


#8 N-DOCOSANE

R.T.: 14.149 min
Delta R.T.: 0.000 min
Response: 2242990
Conc: 16.62 ug/ml

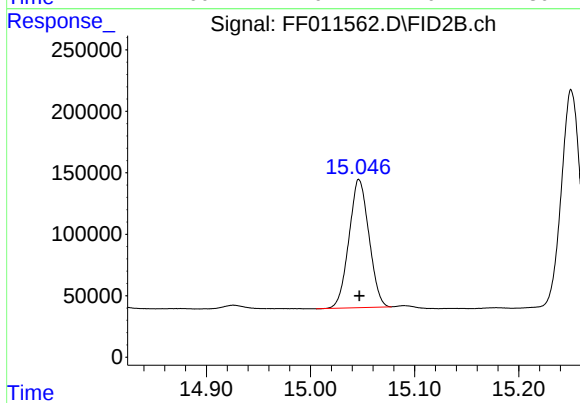

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.047 min
Delta R.T.: 0.000 min
Response: 1391622
Conc: 11.73 ug/ml

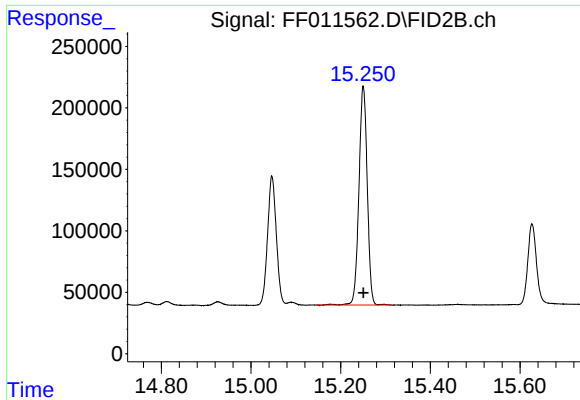

#10 N-TETRACOSANE


R.T.: 15.250 min
Delta R.T.: 0.000 min
Response: 2294238
Conc: 16.92 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MS

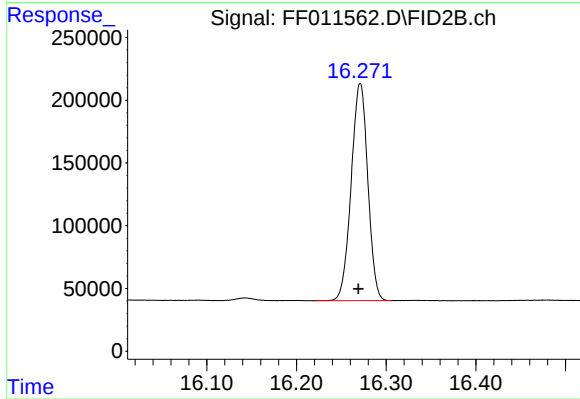

#11 N-HEXACOSANE

R.T.: 16.271 min
Delta R.T.: 0.002 min
Response: 2230135
Conc: 16.69 ug/ml

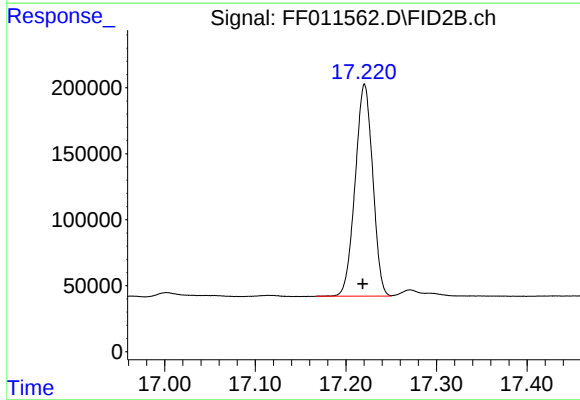

#12 N-OCTACOSANE

R.T.: 17.221 min
Delta R.T.: 0.002 min
Response: 2160925
Conc: 16.31 ug/ml