

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110822\
 Data File : FF011563.D
 Signal(s) : FID2B.ch
 Acq On : 08 Nov 2022 20:40
 Operator : YP\AJ
 Sample : N5494-06MSD
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-17MSD

Integration File: autoint1.e
 Quant Time: Nov 09 05:00:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.048	1373958	11.580 ug/ml
Target Compounds			
2) N-DECANE	4.613	2007642	15.211 ug/ml
3) N-DODECANE	6.773	2088397	15.538 ug/ml
4) N-TETRADECANE	8.597	2172022	16.050 ug/ml
5) N-HEXADECANE	10.202	2273547	16.538 ug/ml
6) N-OCTADECANE	11.642	2295198	16.593 ug/ml
7) N-EICOSANE	12.952	2239895	16.196 ug/ml
8) N-DOCOSANE	14.149	2209957	16.373 ug/ml
10) N-TETRACOSANE	15.250	2236962	16.495 ug/ml
11) N-HEXACOSANE	16.272	2198007	16.452 ug/ml
12) N-OCTACOSANE	17.220	2128559	16.067 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110822\
Data File : FF011563.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2022 20:40
Operator : YP\AJ
Sample : N5494-06MSD
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-17MSD

Integration File: autoint1.e
Quant Time: Nov 09 05:00:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

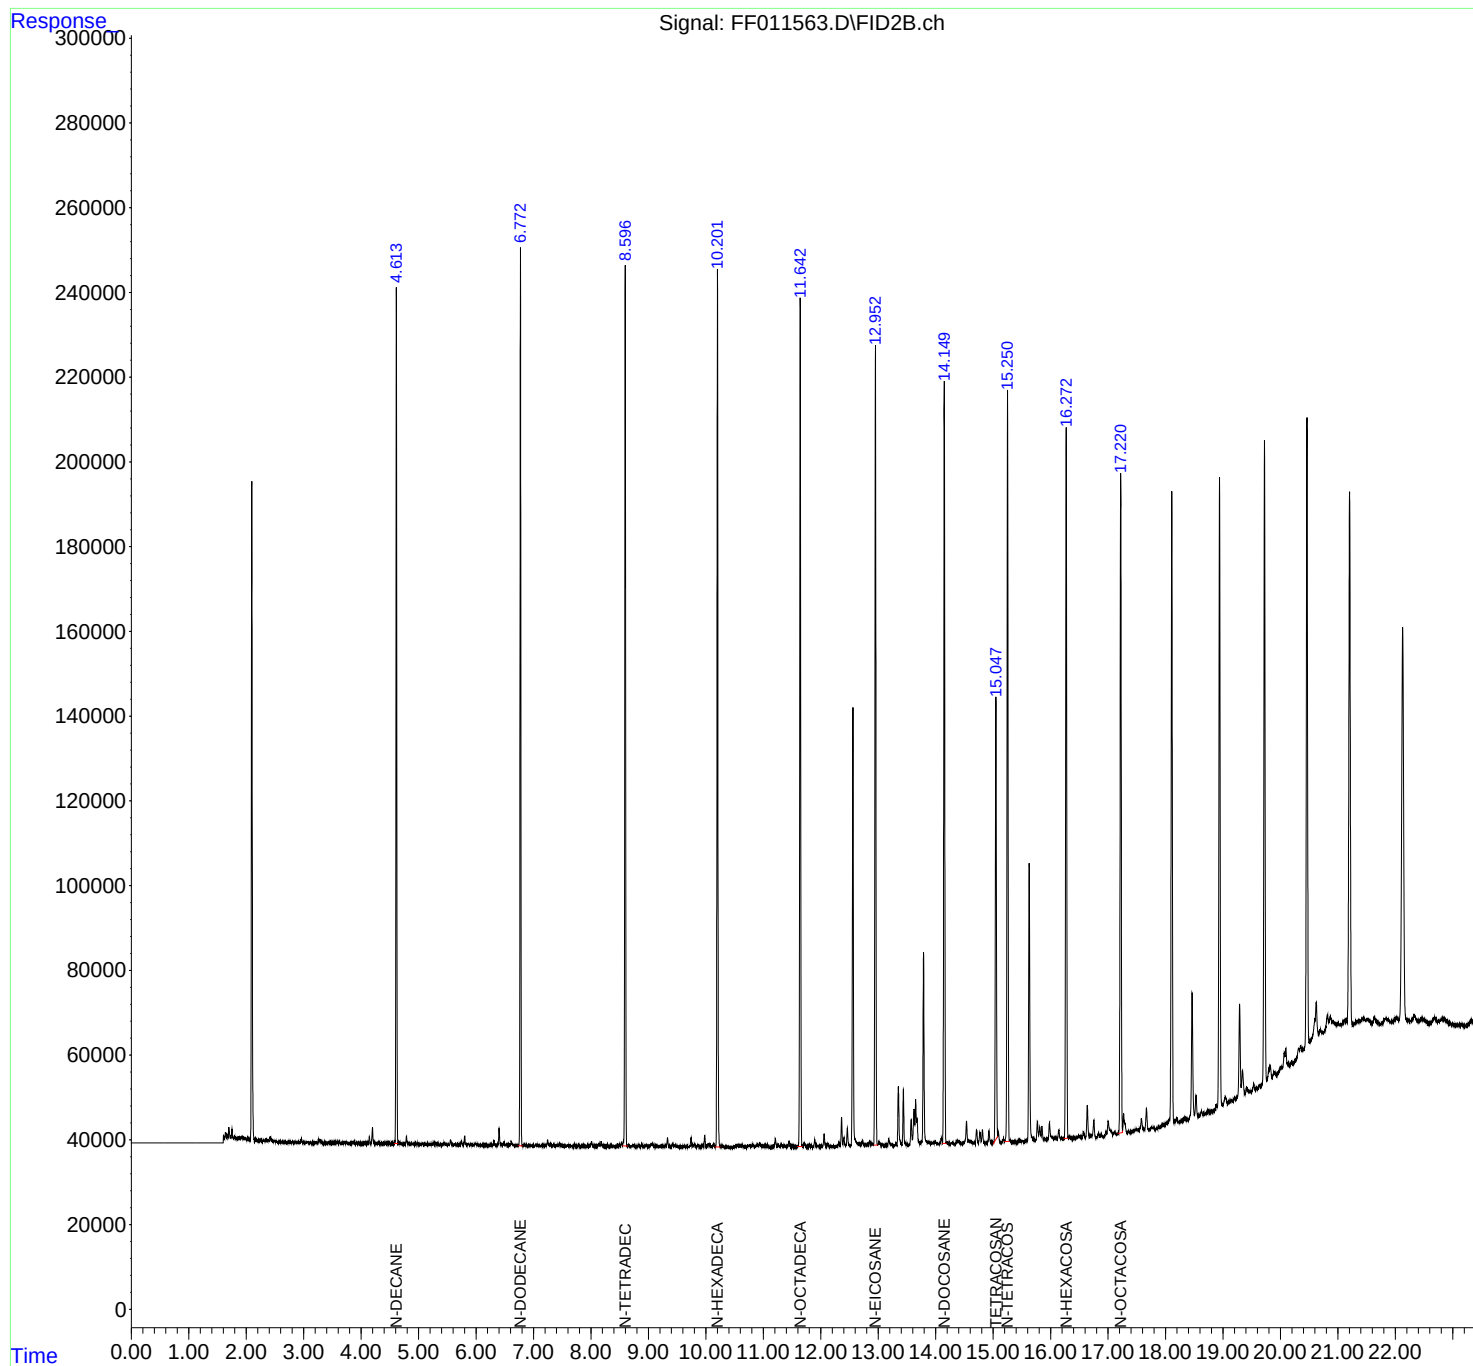


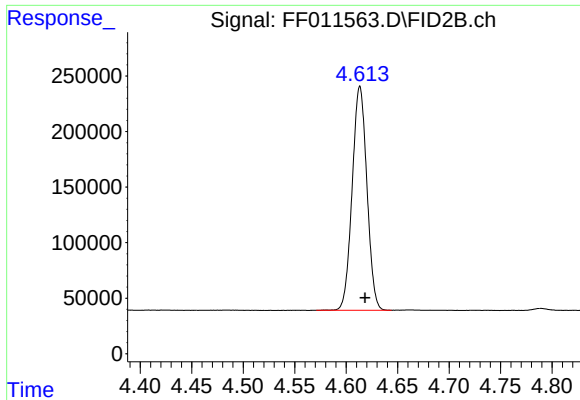

#2 N-DECANE


R.T.: 4.613 min
Delta R.T.: -0.005 min
Response: 2007642
Conc: 15.21 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MSD

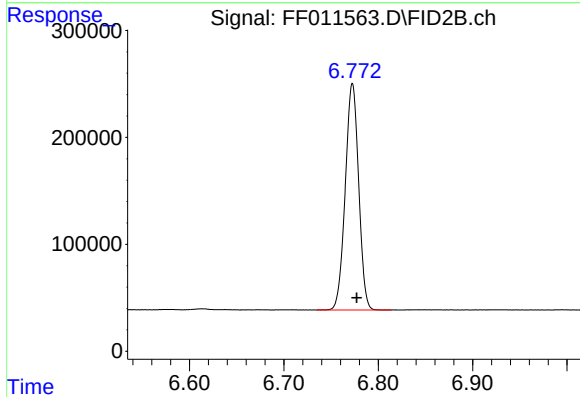


#3 N-DODECANE

R.T.: 6.773 min
Delta R.T.: -0.005 min
Response: 2088397
Conc: 15.54 ug/ml

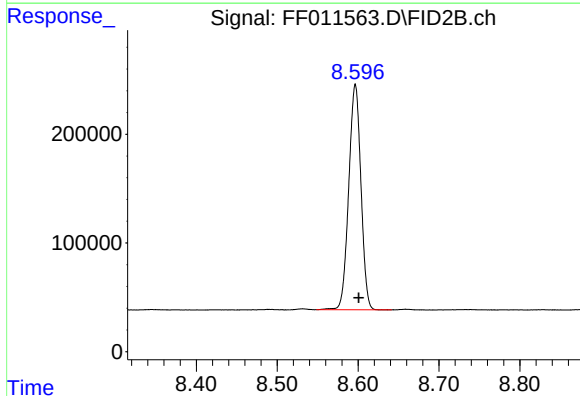


#4 N-TETRADECANE

R.T.: 8.597 min
Delta R.T.: -0.004 min
Response: 2172022
Conc: 16.05 ug/ml

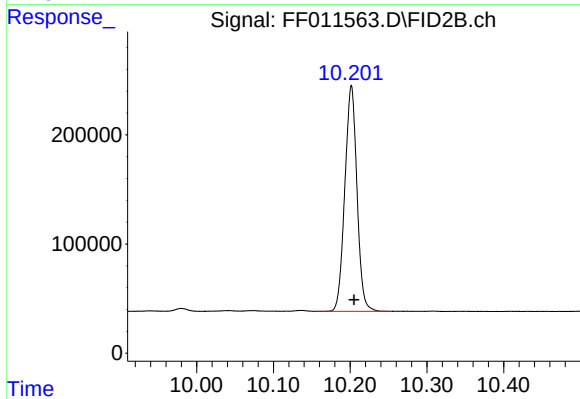

#5 N-HEXADECANE


R.T.: 10.202 min
Delta R.T.: -0.003 min
Response: 2273547
Conc: 16.54 ug/ml

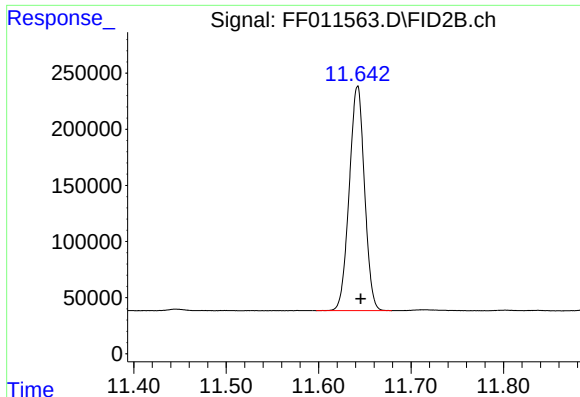

#6 N-OCTADECANE


R.T.: 11.642 min
Delta R.T.: -0.003 min
Response: 2295198
Conc: 16.59 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MSD

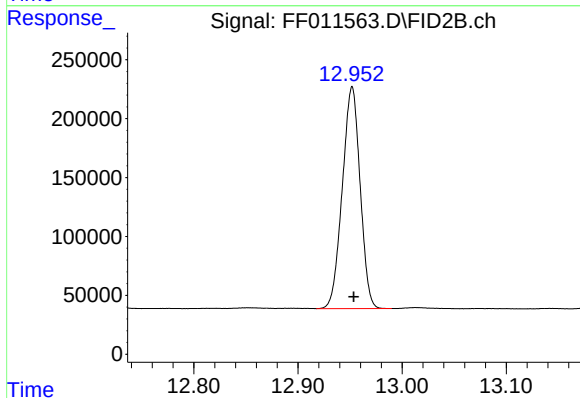


#7 N-EICOSANE

R.T.: 12.952 min
Delta R.T.: -0.001 min
Response: 2239895
Conc: 16.20 ug/ml

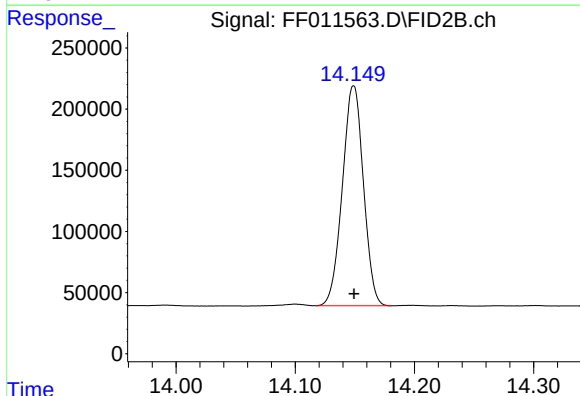


#8 N-DOCOSANE

R.T.: 14.149 min
Delta R.T.: 0.000 min
Response: 2209957
Conc: 16.37 ug/ml

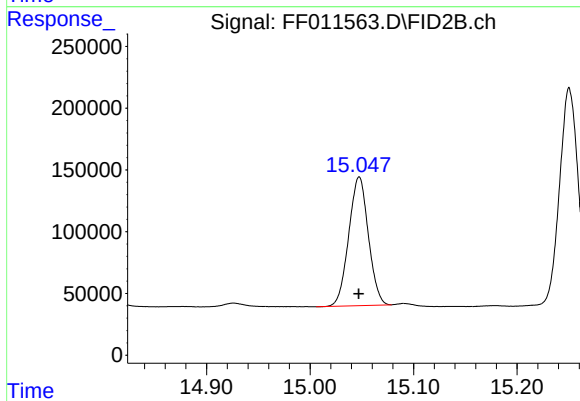

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.048 min
Delta R.T.: 0.000 min
Response: 1373958
Conc: 11.58 ug/ml

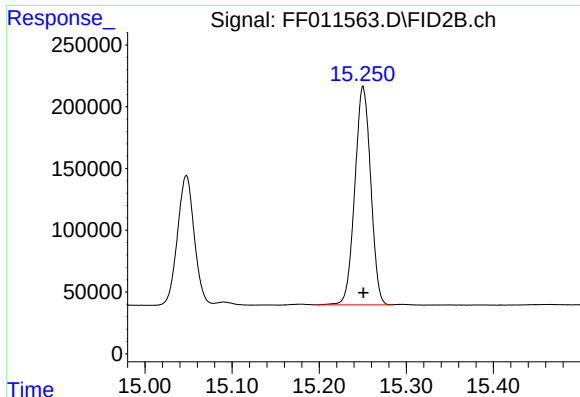

#10 N-TETRACOSANE


R.T.: 15.250 min
Delta R.T.: 0.000 min
Response: 2236962
Conc: 16.50 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-17MSD

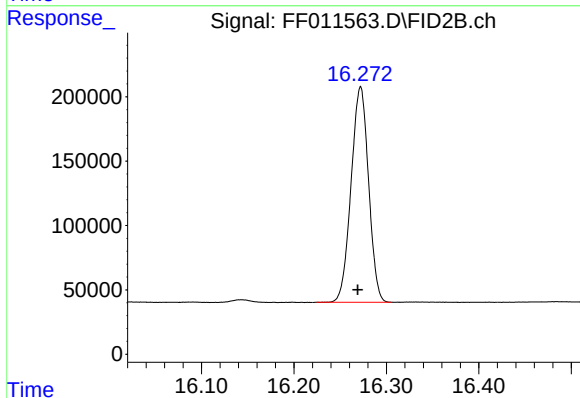

#11 N-HEXACOSANE

R.T.: 16.272 min
Delta R.T.: 0.003 min
Response: 2198007
Conc: 16.45 ug/ml

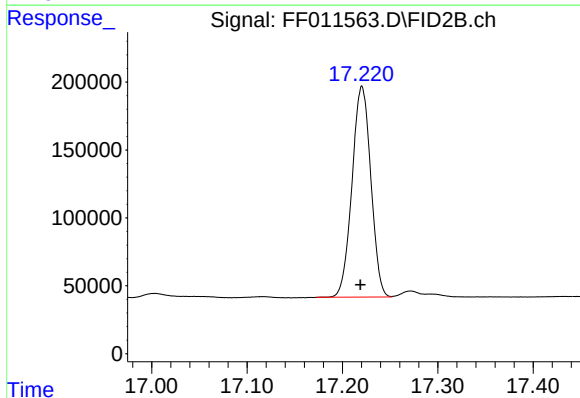

#12 N-OCTACOSANE

R.T.: 17.220 min
Delta R.T.: 0.002 min
Response: 2128559
Conc: 16.07 ug/ml