

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110824AR\
Data File : FF014986.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2024 22:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 00:29:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 110724.M
Quant Title : GC Extractables
QLast Update : Fri Nov 08 08:49:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	Indeno[1,2,3-cd]pyren...	18.502	177950	1.295 ug/ml
20) T	Dibenz[a,h]anthracene...	18.502	177950	1.203 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110824AR\
Data File : FF014986.D
Signal(s) : FID2B.ch
Acq On : 08 Nov 2024 22:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 00:29:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 110724.M
Quant Title : GC Extractables
QLast Update : Fri Nov 08 08:49:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

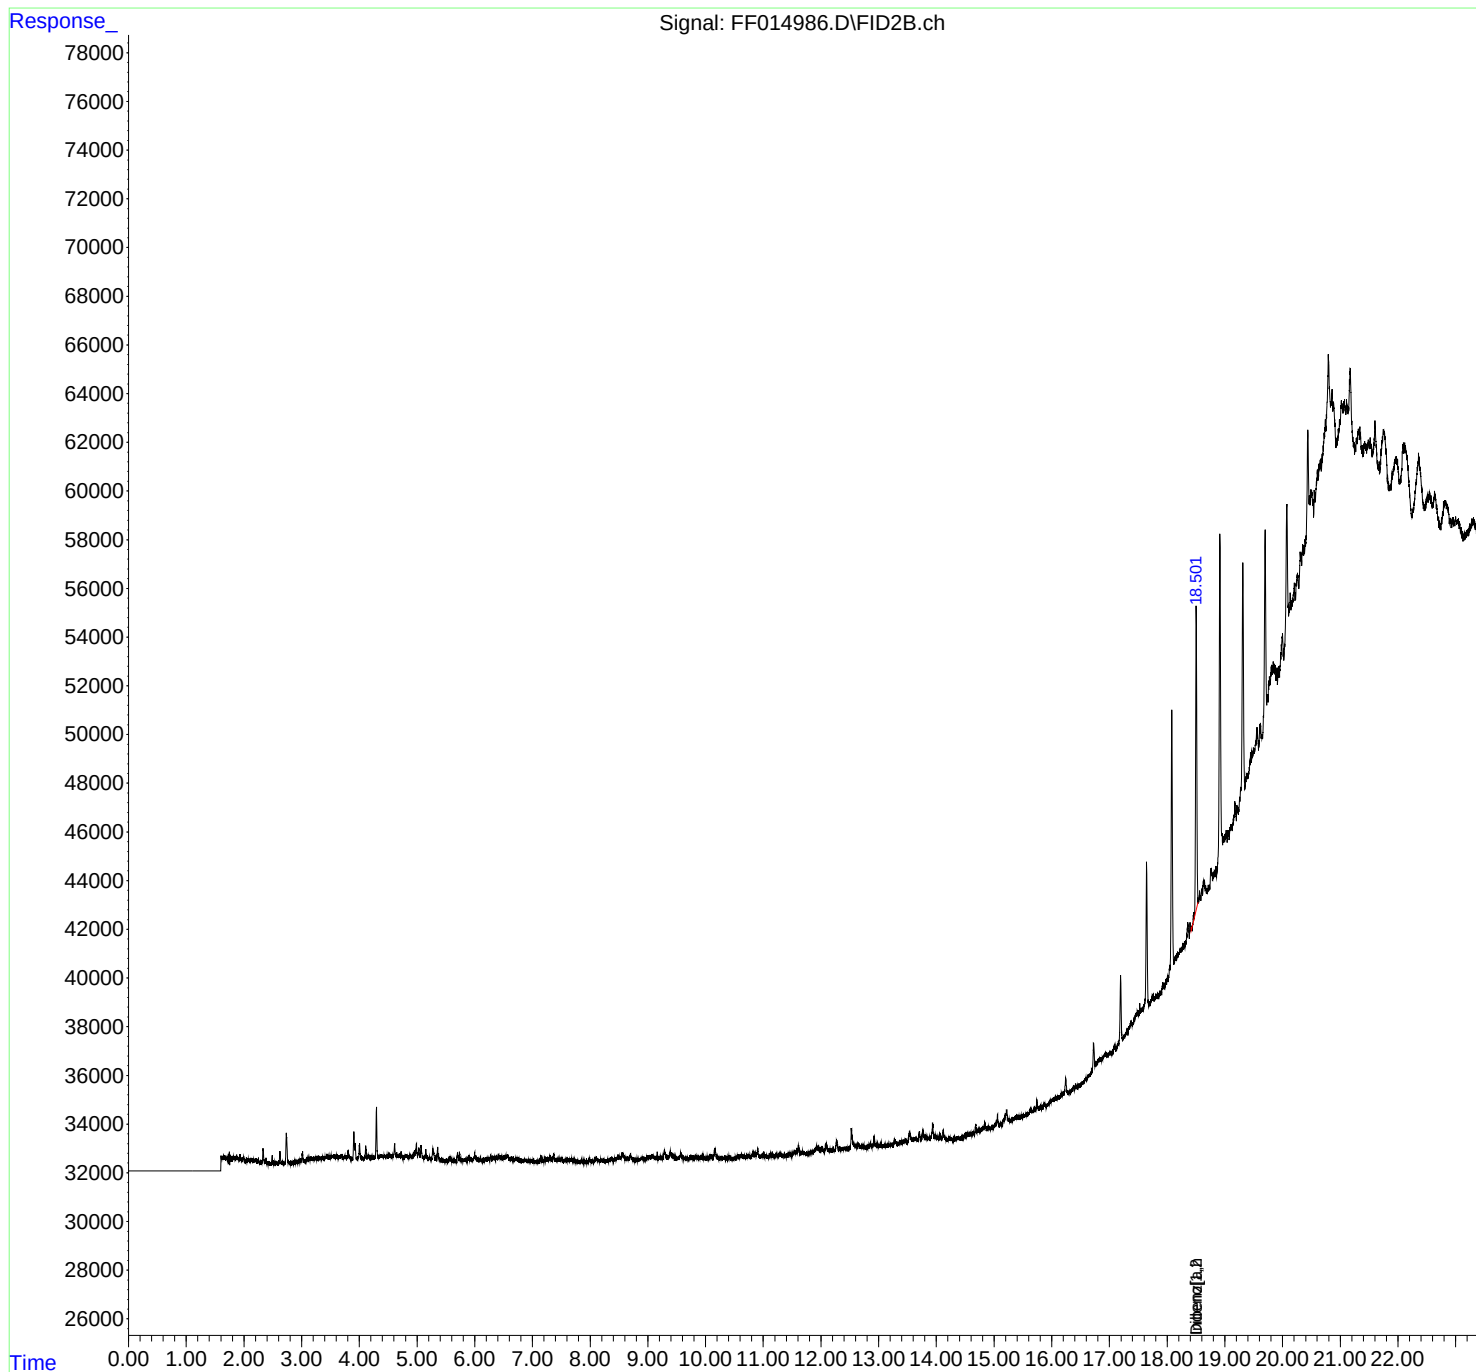


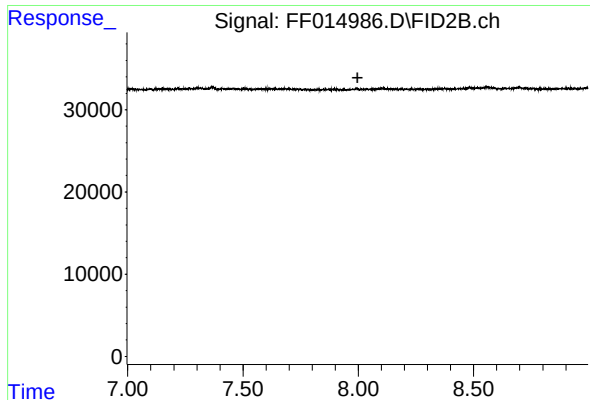

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.997 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

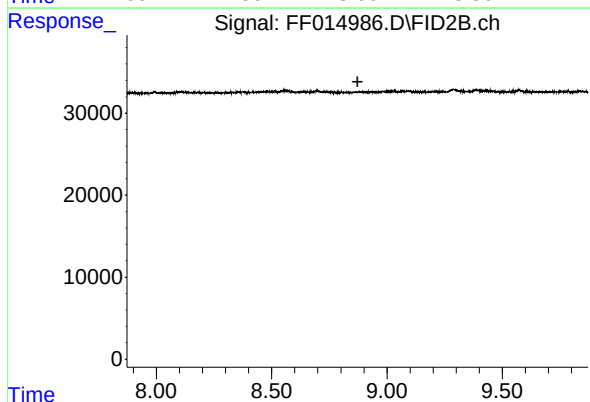


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

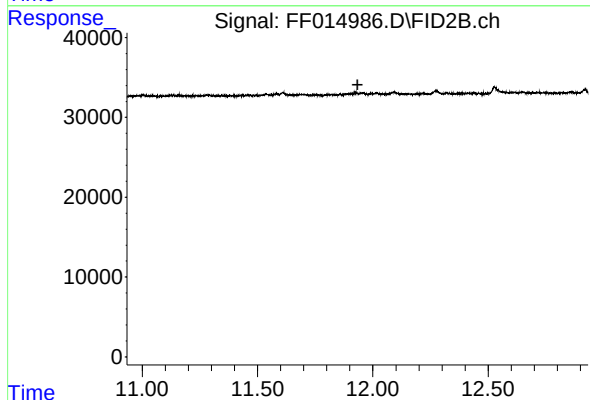


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.933 min
Response: 0
Conc: N.D.

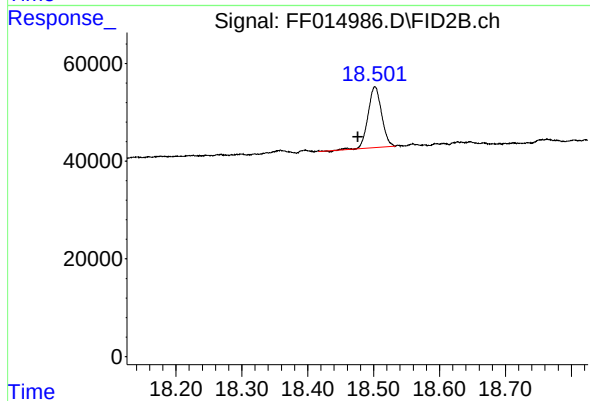

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.502 min
Delta R.T.: 0.026 min
Response: 177950
Conc: 1.29 ug/ml

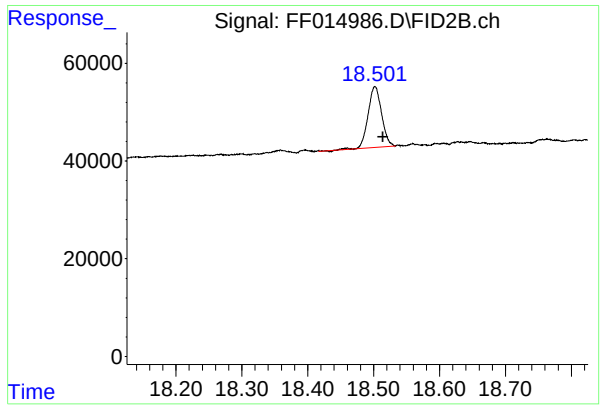

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.502 min

Delta R.T.: -0.012 min

Response: 177950

Conc: 1.20 ug/ml

Instrument :

FID_F

ClientSampleId :