

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110920\
Data File : FF007818.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2020 11:42
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:47:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.458	6143503	44.384 ug/ml
12)	N-OCTACOSANE	16.900	5821505	42.920 ug/ml
13)	N-TRIACONTANE	17.786	428889	3.315 ug/ml
14)	N-DOTRIACONTANE	18.621	523425	4.515 ug/ml
15)	N-TETRATRIACONTANE	19.406	373239	3.974 ug/ml
16)	N-HEXATRIACONTANE	20.149	141440	1.862 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110920\
Data File : FF007818.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2020 11:42
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:47:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

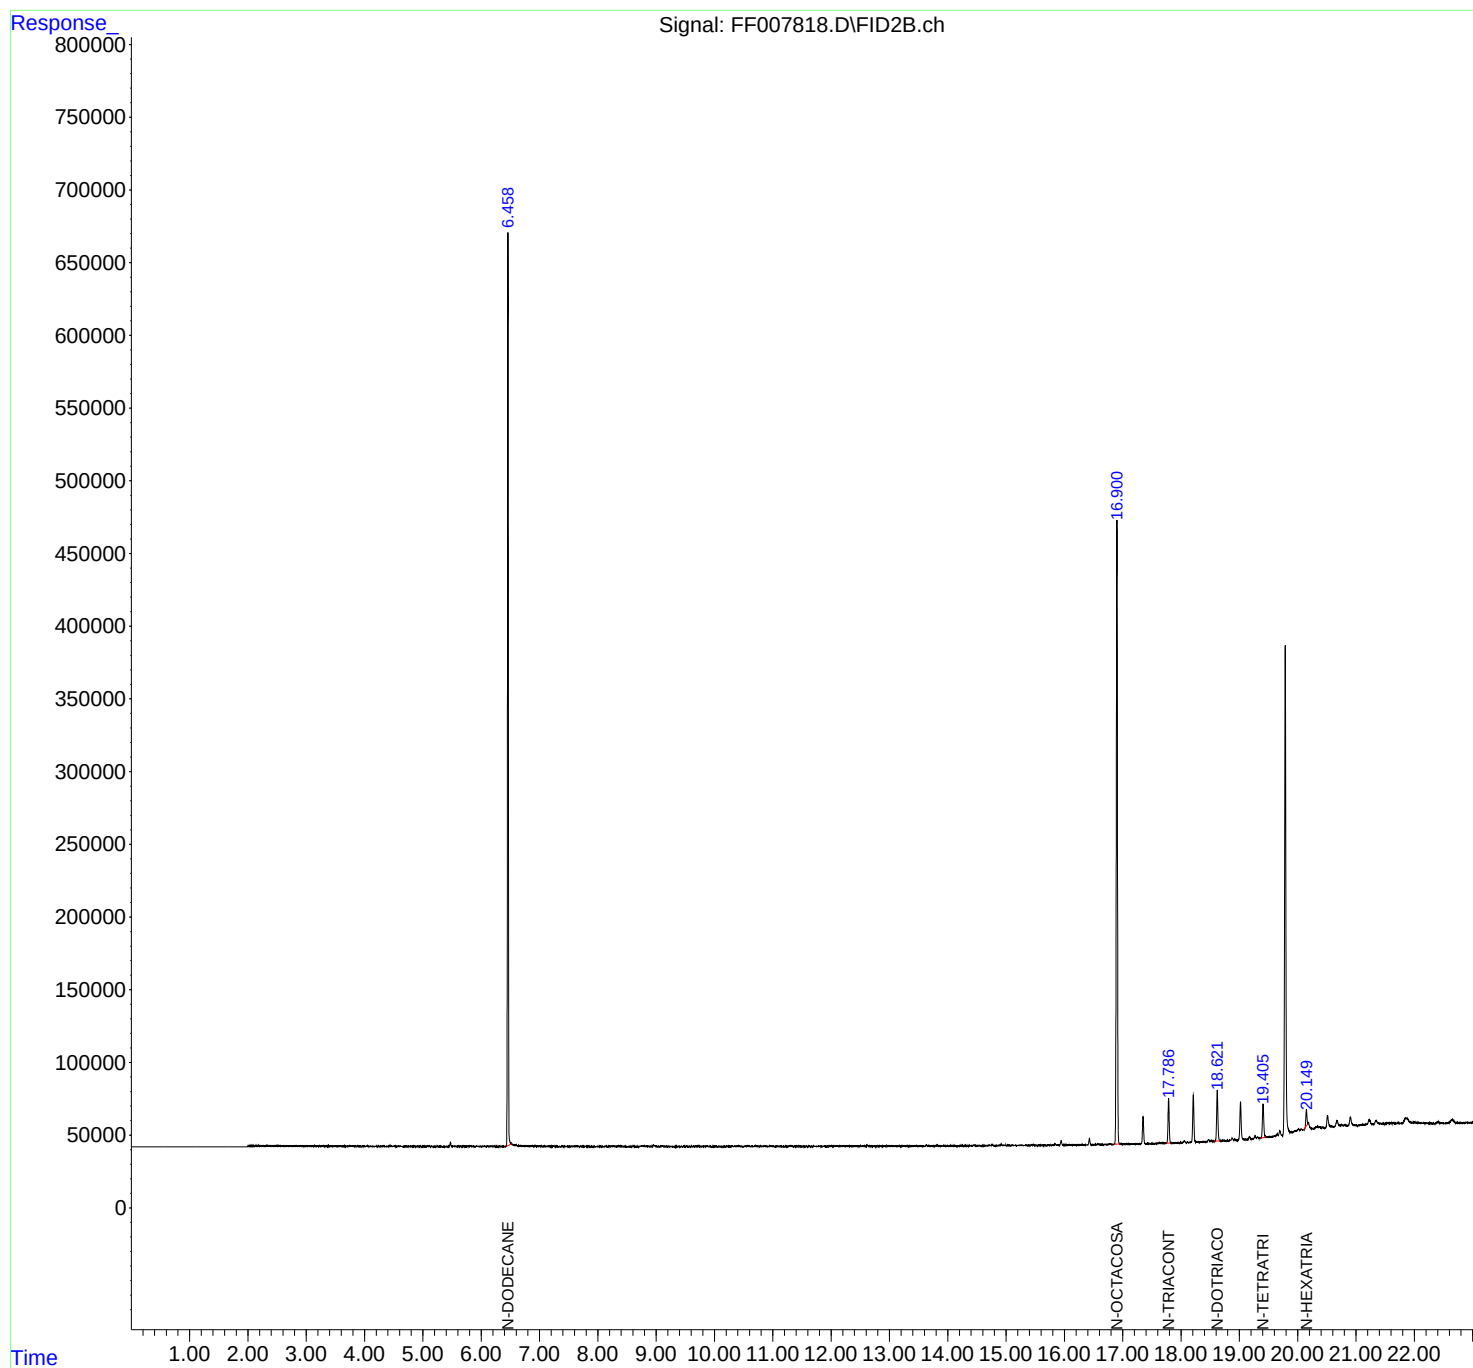


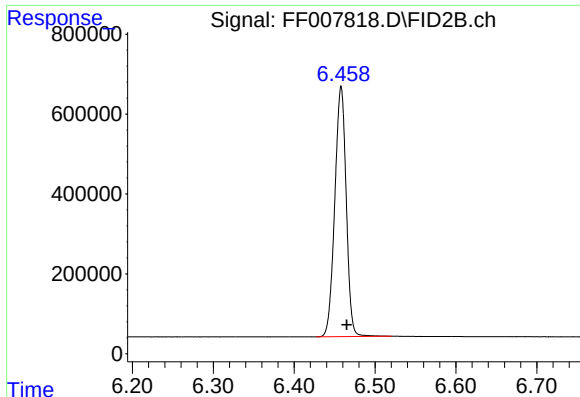

#3 N-DODECANE


R.T.: 6.458 min
Delta R.T.: -0.007 min
Response: 6143503
Conc: 44.38 ug/ml

Instrument :
FID_F
ClientSampleId :

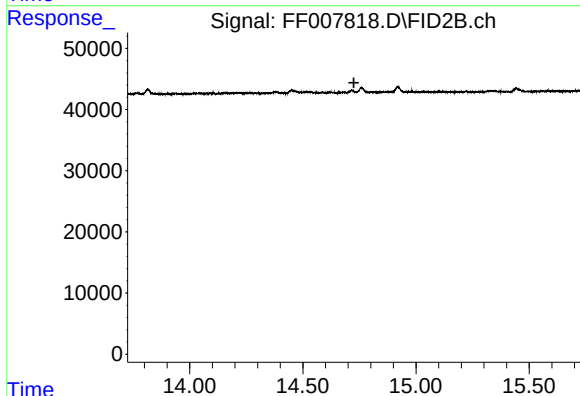


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.726 min
Response: 0
Conc: N.D.

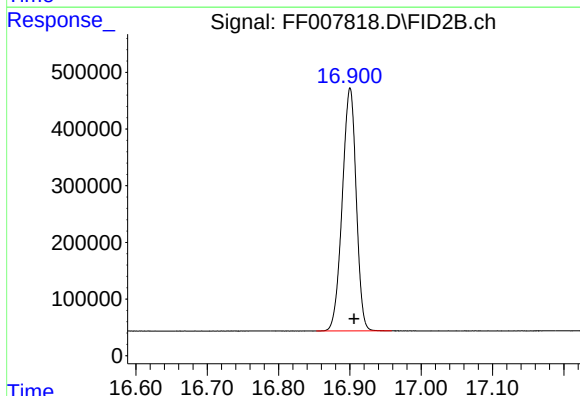


#12 N-OCTACOSANE

R.T.: 16.900 min
Delta R.T.: -0.006 min
Response: 5821505
Conc: 42.92 ug/ml

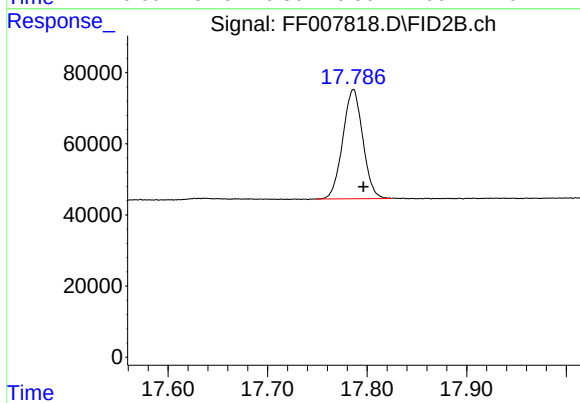

#13 N-TRIACONTANE


R.T.: 17.786 min
Delta R.T.: -0.010 min
Response: 428889
Conc: 3.31 ug/ml

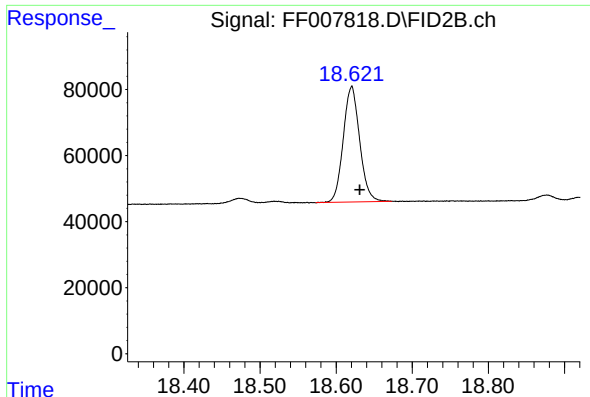

#14 N-DOTRIACONTANE


R.T.: 18.621 min
Delta R.T.: -0.011 min
Response: 523425
Conc: 4.52 ug/ml

Instrument :
FID_F
ClientSampleId :

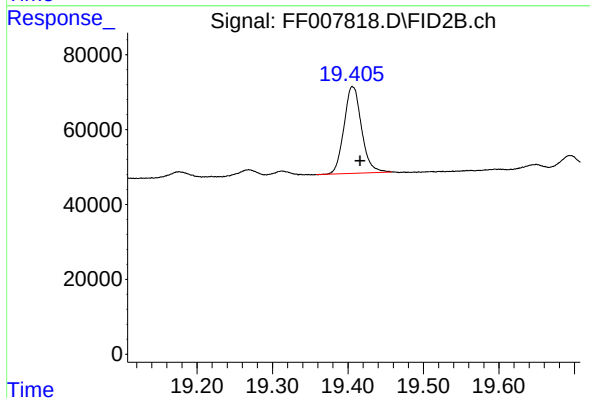

#15 N-TETRATRIACONTANE

R.T.: 19.406 min
Delta R.T.: -0.010 min
Response: 373239
Conc: 3.97 ug/ml

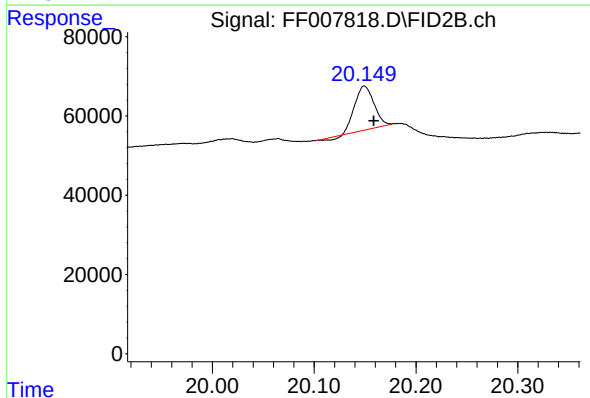

#16 N-HEXATRIACONTANE

R.T.: 20.149 min
Delta R.T.: -0.009 min
Response: 141440
Conc: 1.86 ug/ml