

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110920\
Data File : FF007828.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2020 19:24
Operator : DD\AJ
Sample : L4668-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:50:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.716	2363339	18.502 ug/ml
Target Compounds			
4) N-TETRADECANE	8.320f	106490	0.754 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110920\
Data File : FF007828.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2020 19:24
Operator : DD\AJ
Sample : L4668-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:50:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

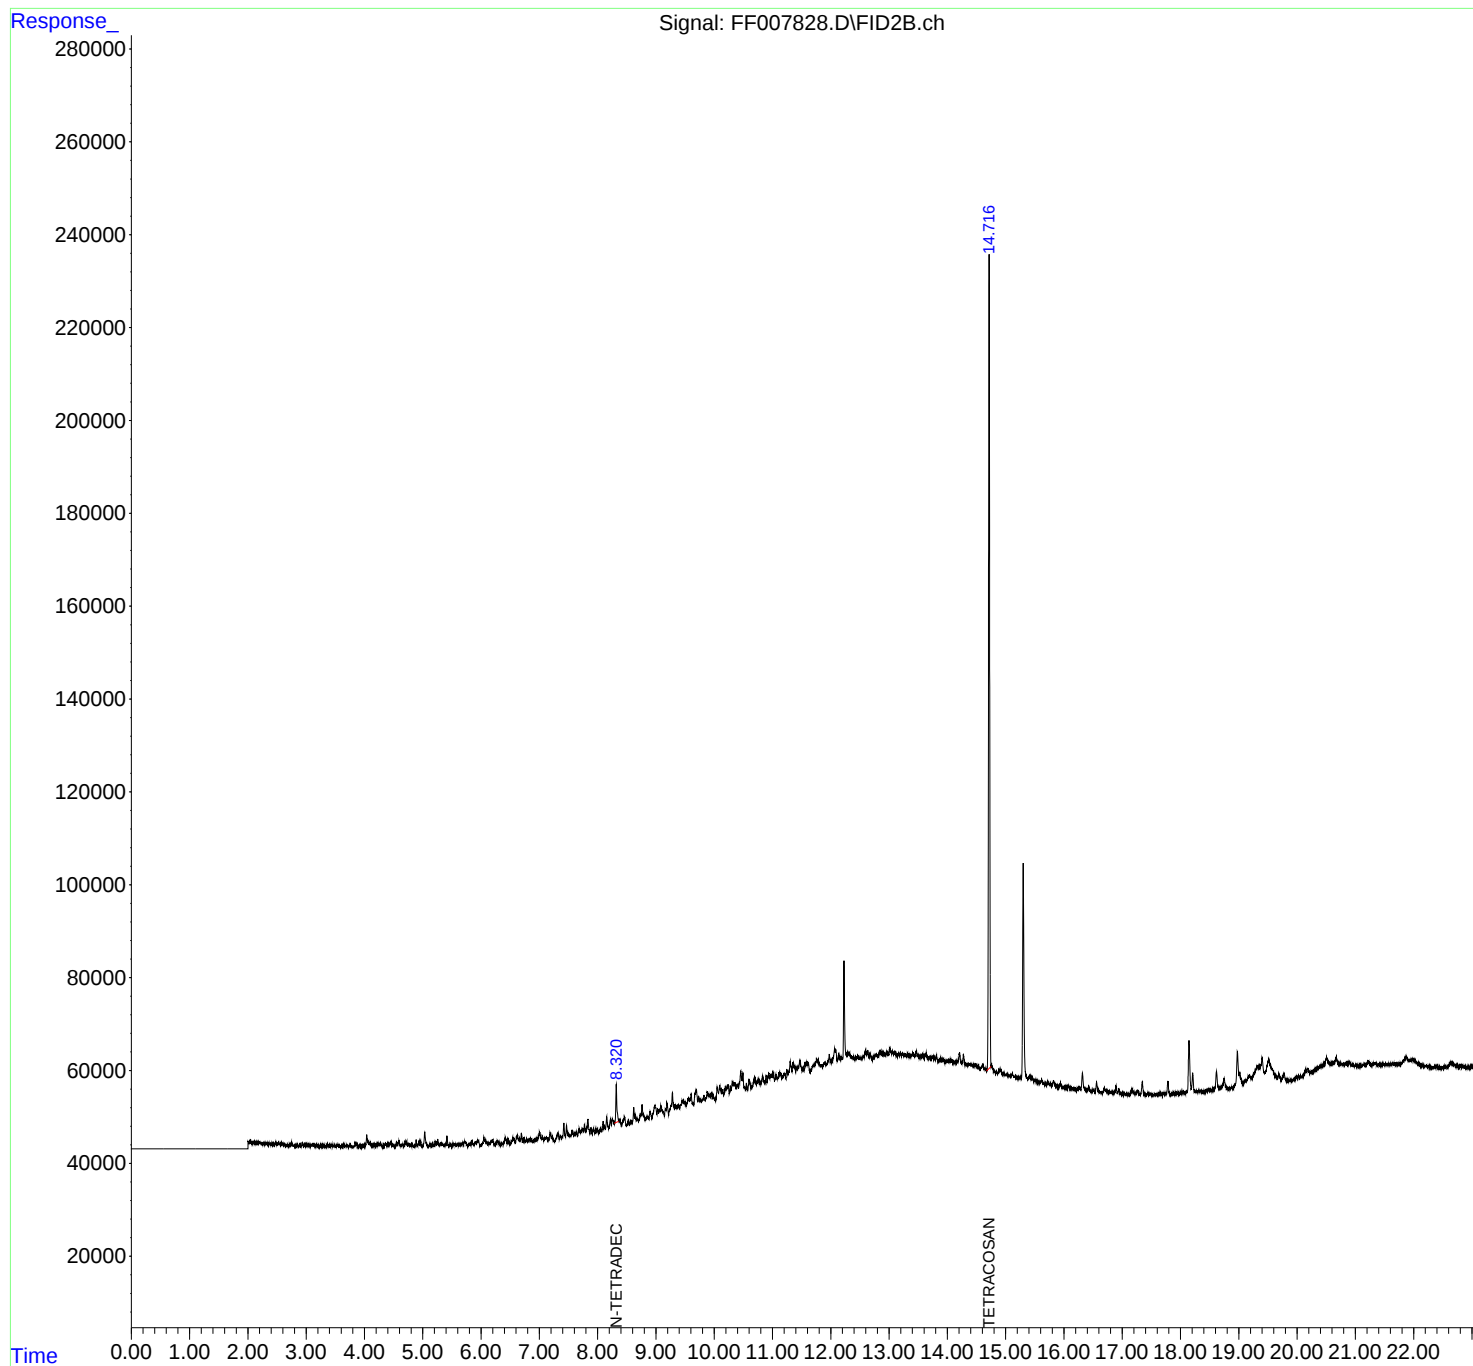


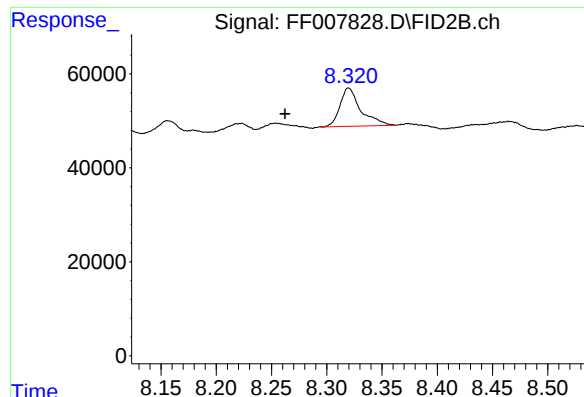

#4 N-TETRADECANE

R.T.: 8.320 min
Delta R.T.: 0.058 min
Response: 106490
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

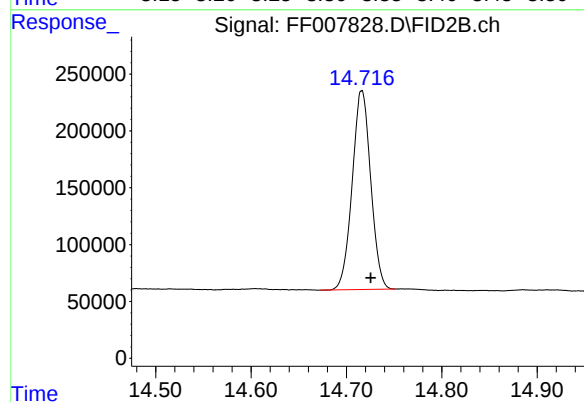

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.716 min
Delta R.T.: -0.009 min
Response: 2363339
Conc: 18.50 ug/ml