

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110920\
Data File : FF007836.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2020 23:31
Operator : DD\AJ
Sample : L4668-08
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:51:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.715	2525799	19.774 ug/ml
Target Compounds			
3) N-DODECANE	6.480	79467	0.574 ug/ml
4) N-TETRADECANE	8.220	83768	0.593 ug/ml
12) N-OCTACOSANE	16.942	933767	6.884 ug/ml
14) N-DOTRIACONTANE	18.614	92741	0.800 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110920\
Data File : FF007836.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2020 23:31
Operator : DD\AJ
Sample : L4668-08
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:51:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

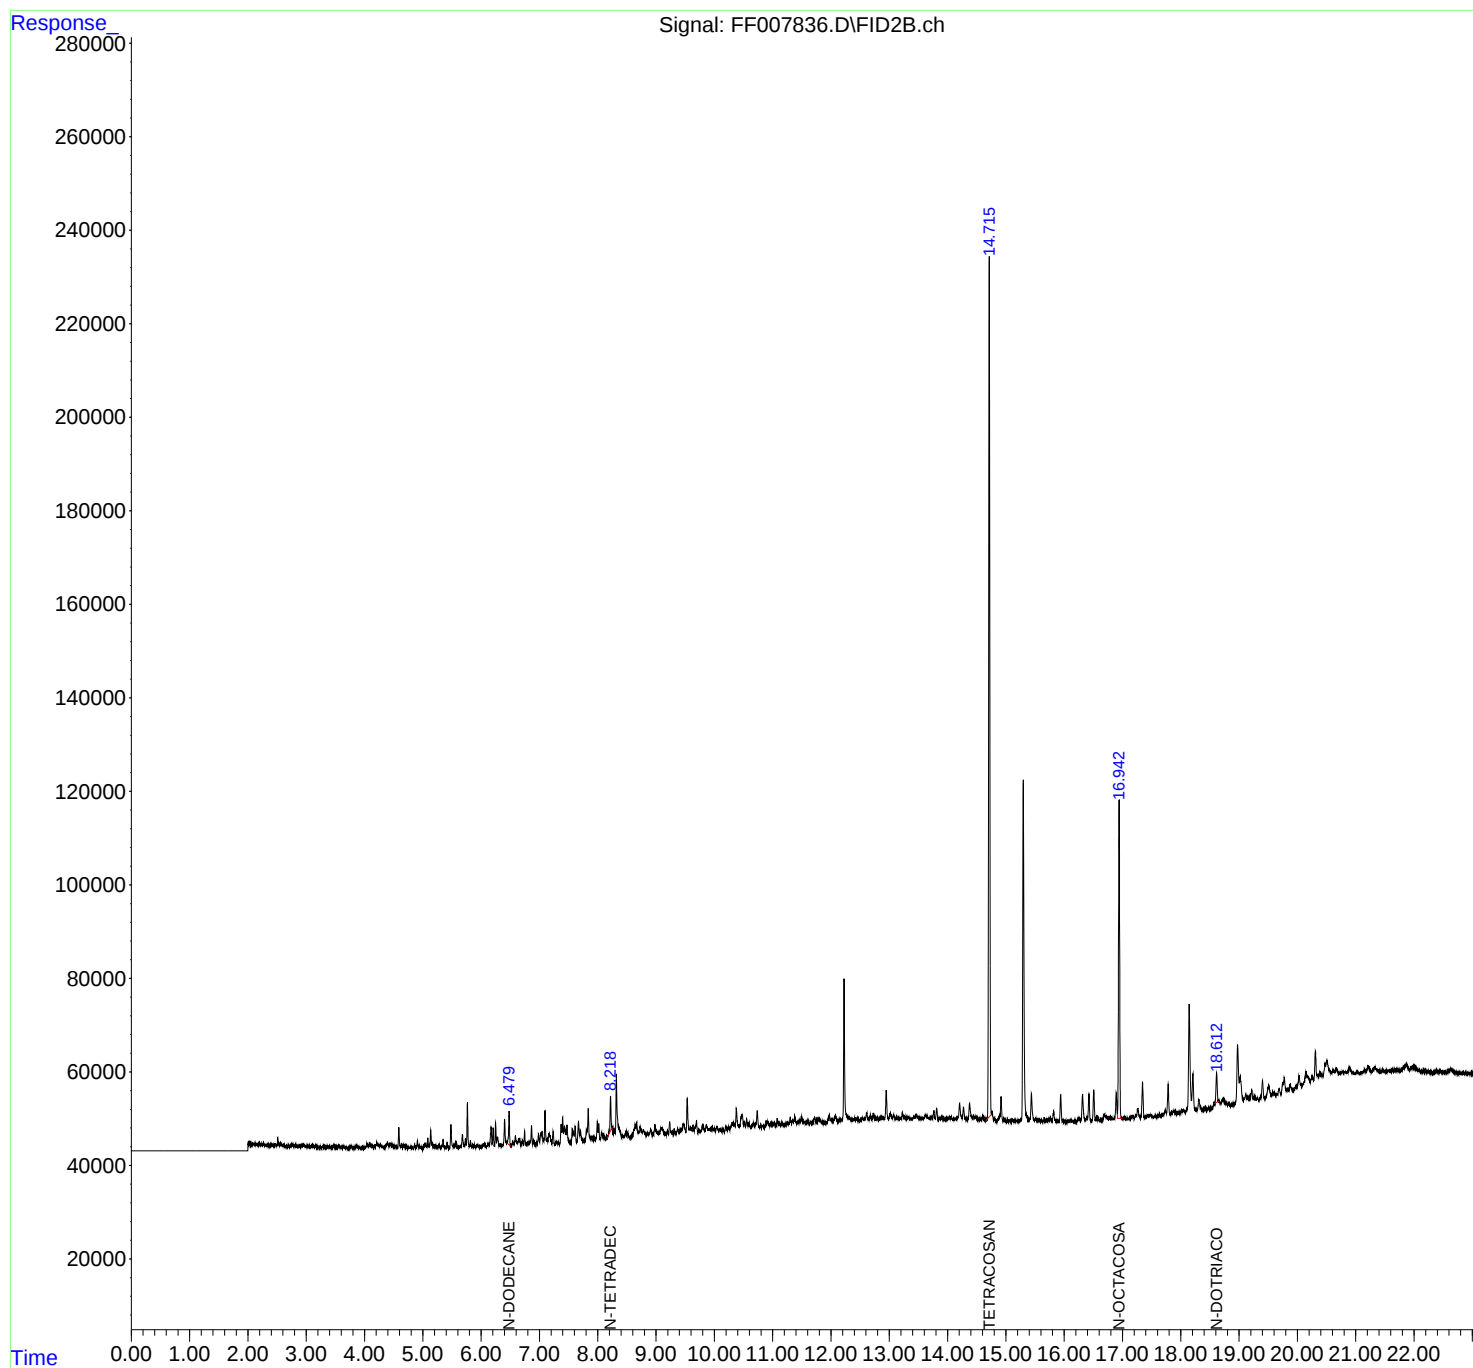


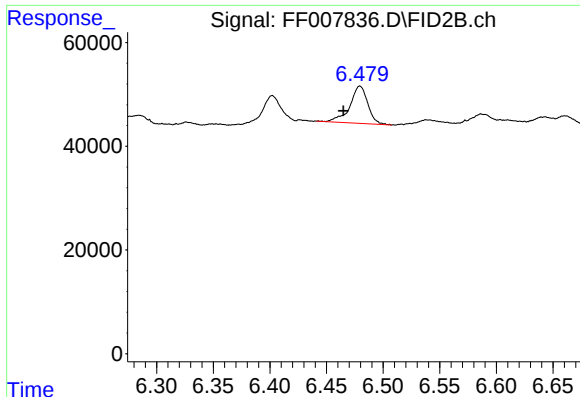

#3 N-DODECANE


R.T.: 6.480 min
Delta R.T.: 0.015 min
Response: 79467
Conc: 0.57 ug/ml

Instrument :
FID_F
ClientSampleId :

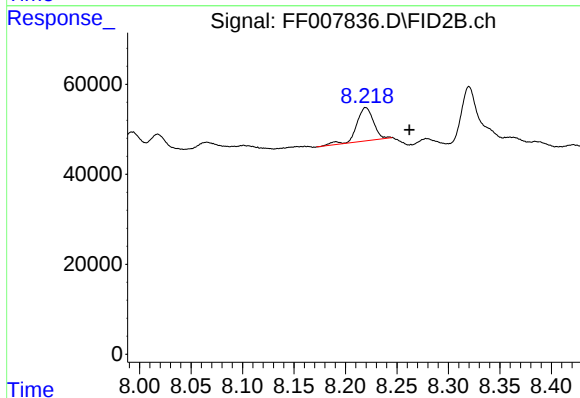


#4 N-TETRADECANE

R.T.: 8.220 min
Delta R.T.: -0.043 min
Response: 83768
Conc: 0.59 ug/ml

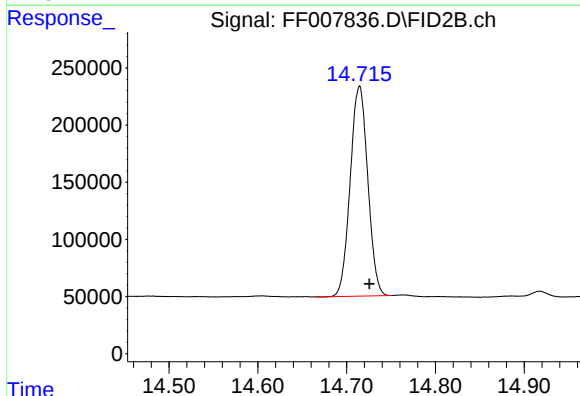


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: -0.011 min
Response: 2525799
Conc: 19.77 ug/ml

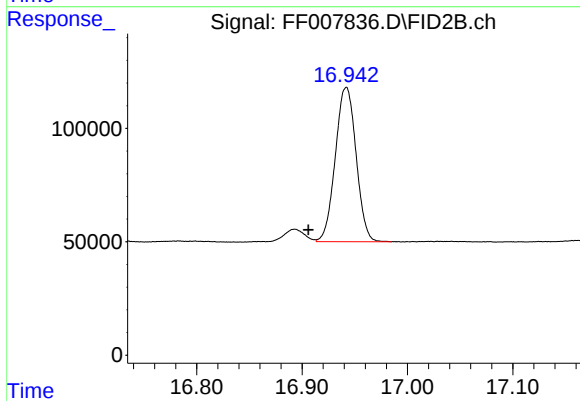

#12 N-OCTACOSANE

R.T.: 16.942 min
Delta R.T.: 0.036 min
Response: 933767
Conc: 6.88 ug/ml

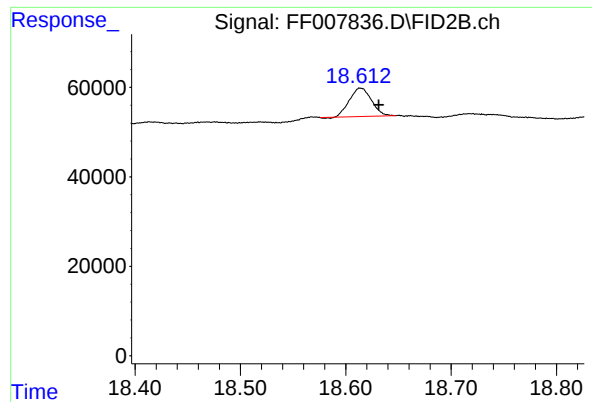

#14 N-DOTRIACONTANE

R.T.: 18.614 min
Delta R.T.: -0.017 min
Response: 92741
Conc: 0.80 ug/ml

Instrument :
FID_F
ClientSampleId :