

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009299.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 09:08
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 14:23:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.594	345997	3.231 ug/ml
16)	N-HEXATRIACONTANE	20.129	235799	2.319 ug/ml
18)	N-TETRACONTANE	21.767	567157	5.879 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009299.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 09:08
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 14:23:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

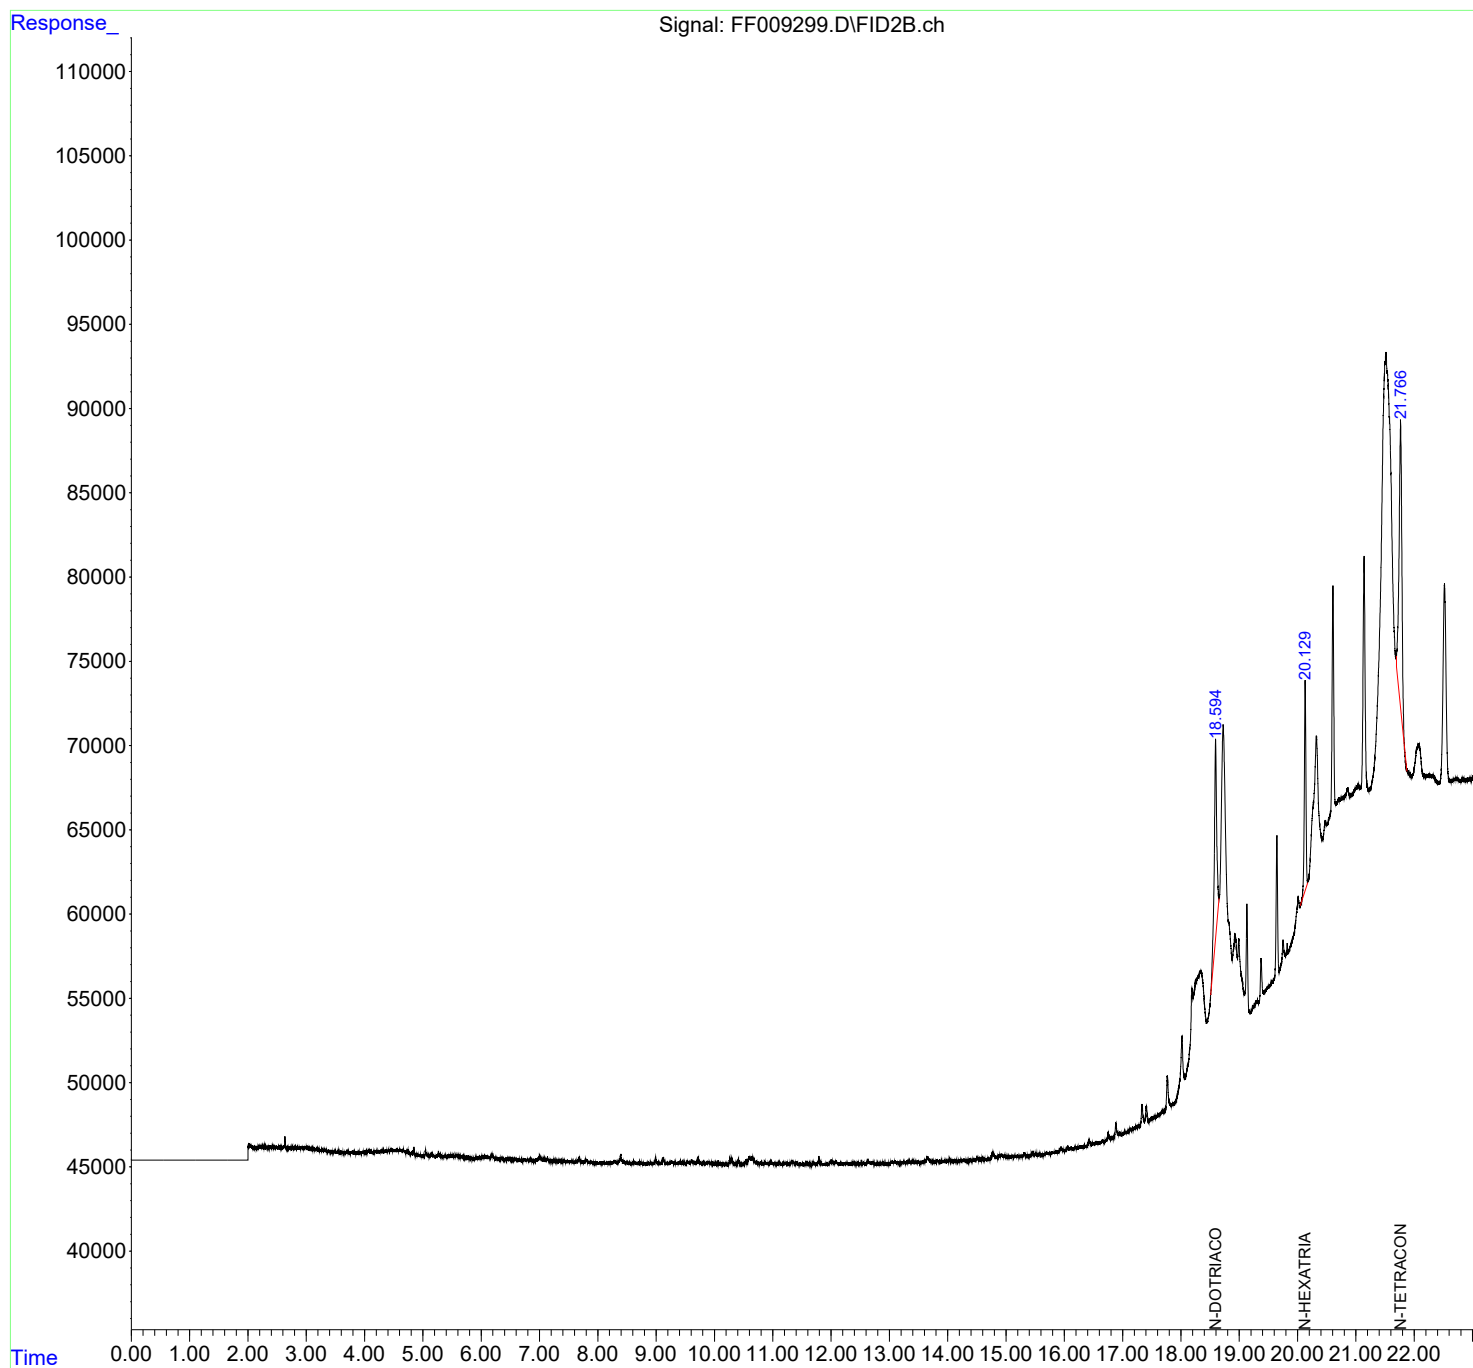


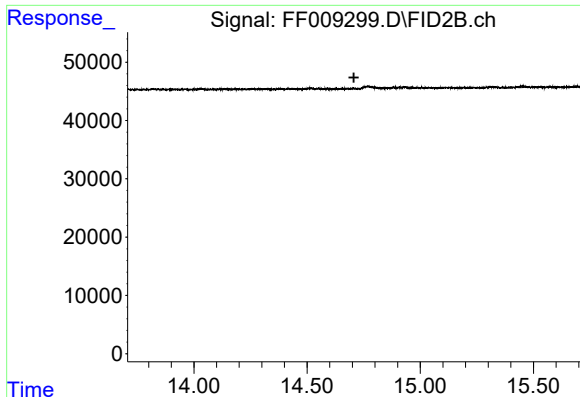

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.707 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

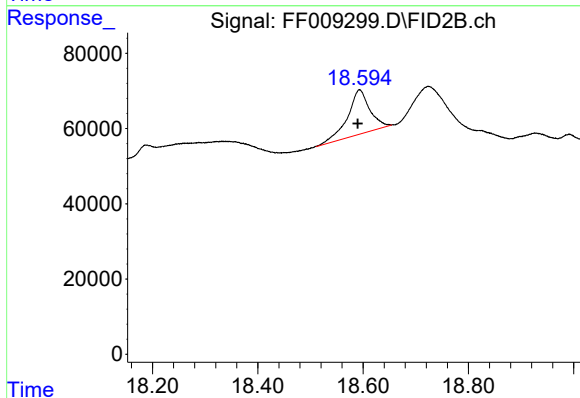


#14 N-DOTRIACONTANE

R.T.: 18.594 min
Delta R.T.: 0.004 min
Response: 345997
Conc: 3.23 ug/ml

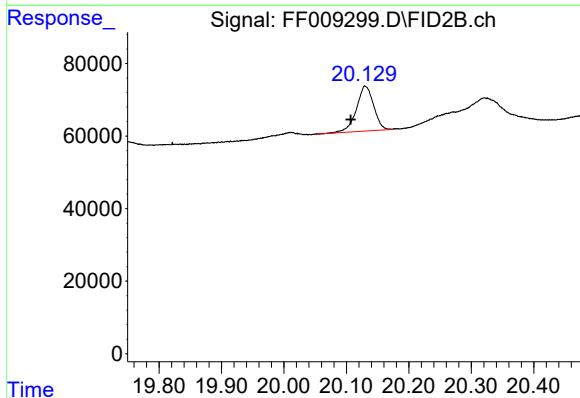

#16 N-HEXATRIACONTANE

R.T.: 20.129 min
Delta R.T.: 0.022 min
Response: 235799
Conc: 2.32 ug/ml

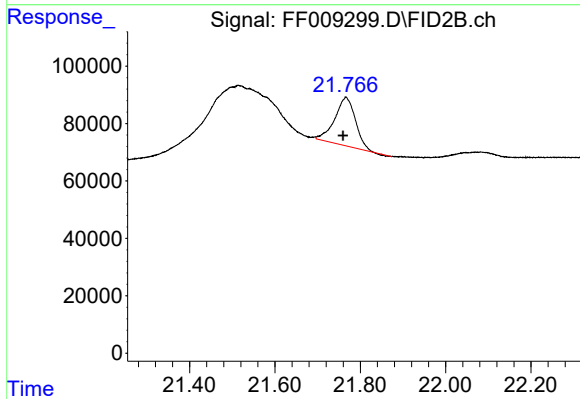

#18 N-TETRACONTANE

R.T.: 21.767 min
Delta R.T.: 0.007 min
Response: 567157
Conc: 5.88 ug/ml