

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
 Data File : FF009310.D
 Signal(s) : FID2B.ch
 Acq On : 09 Nov 2021 15:48
 Operator : AJ\MA
 Sample : M4507-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 10 00:56:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
 Quant Title :
 QLast Update : Tue Nov 09 14:23:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.703	1726769	15.434 ug/ml
Target Compounds			
4) N-TETRADECANE	8.234	191630	1.415 ug/ml
14) N-DOTRIACONTANE	18.591	162937	1.521 ug/ml
16) N-HEXATRIACONTANE	20.135	193994	1.908 ug/ml
18) N-TETRACONTANE	21.772	468990	4.861 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009310.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 15:48
Operator : AJ\MA
Sample : M4507-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:56:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

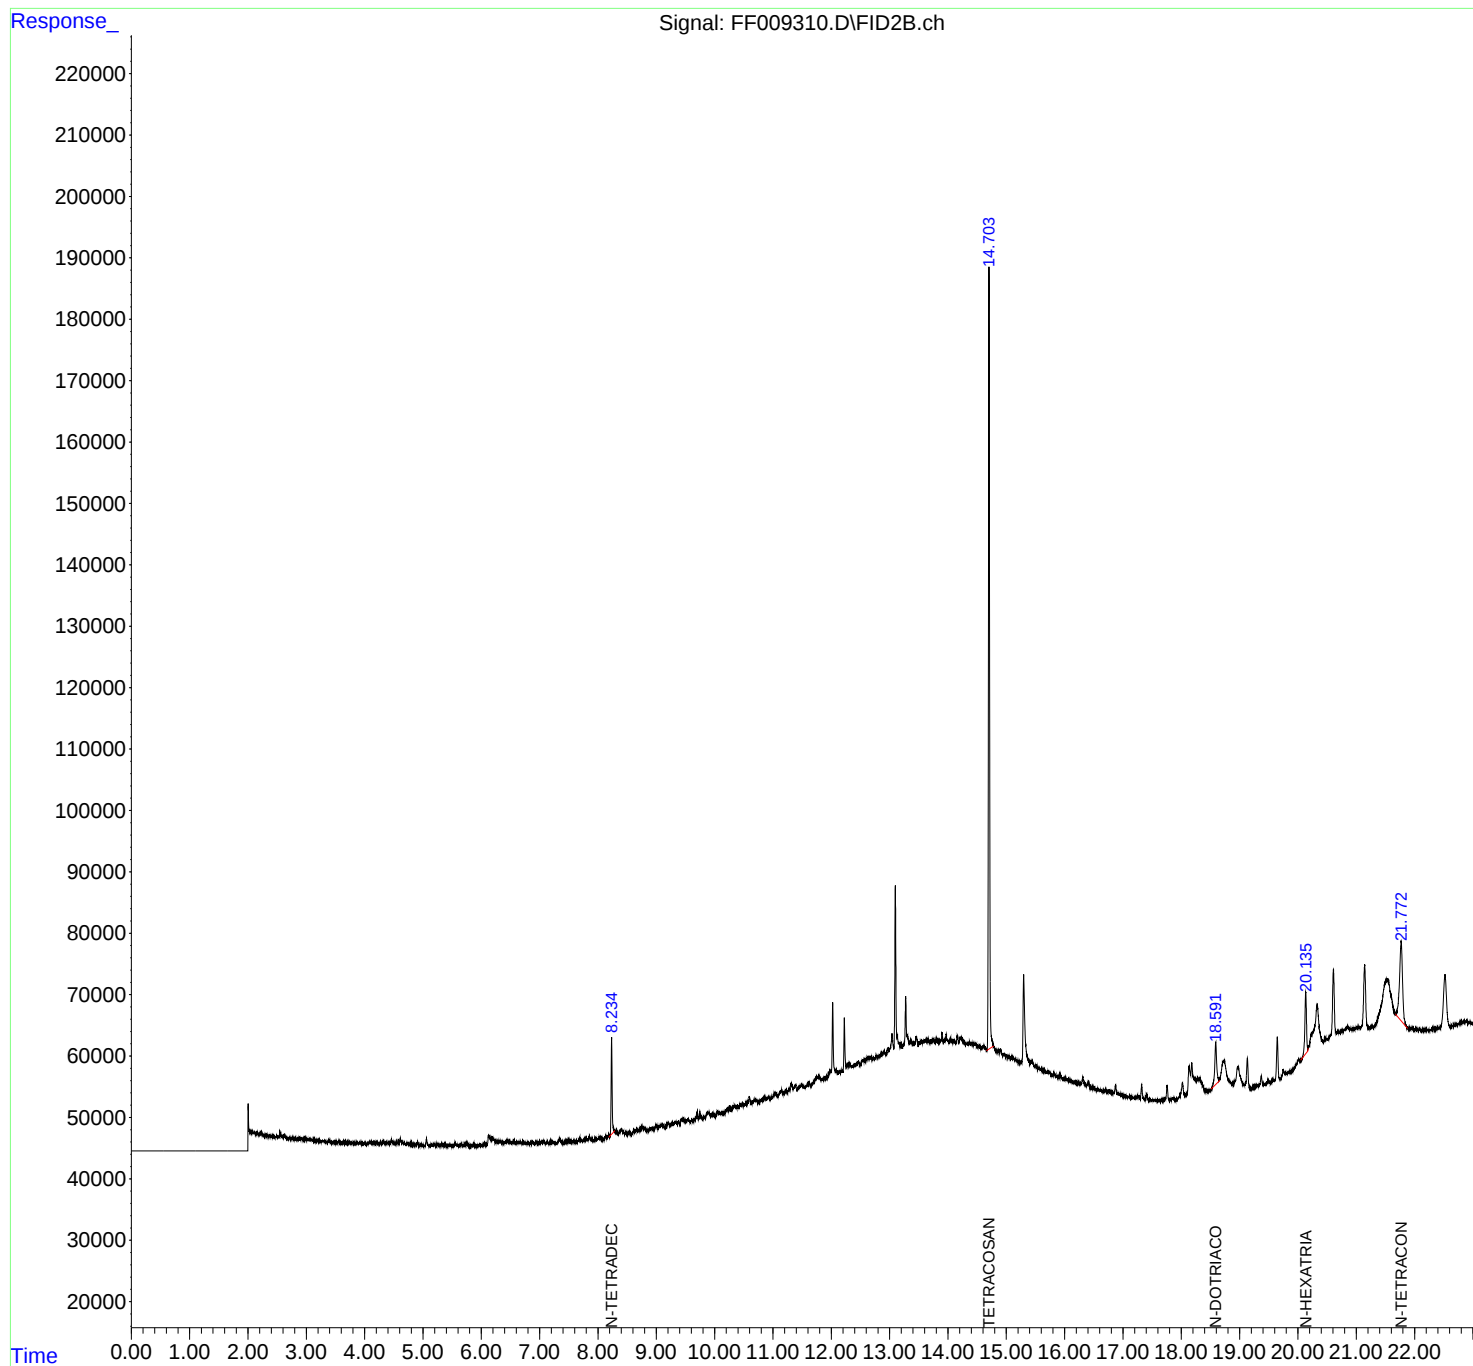


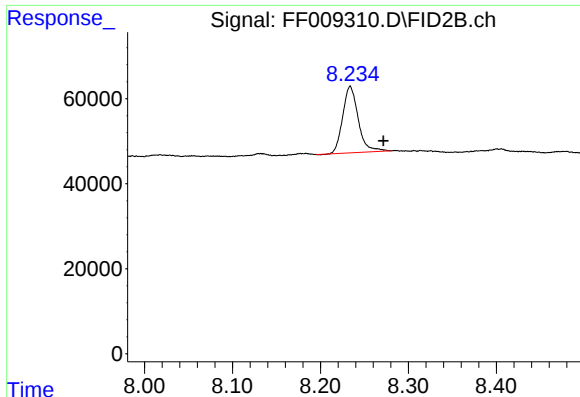

#4 N-TETRADECANE


R.T.: 8.234 min
Delta R.T.: -0.038 min
Response: 191630
Conc: 1.42 ug/ml

Instrument :
FID_F
ClientSampleId :

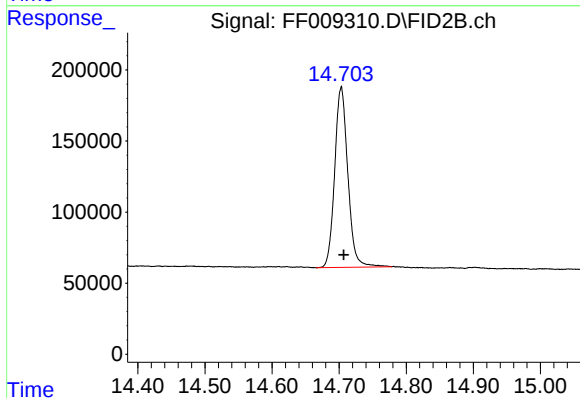


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.703 min
Delta R.T.: -0.003 min
Response: 1726769
Conc: 15.43 ug/ml

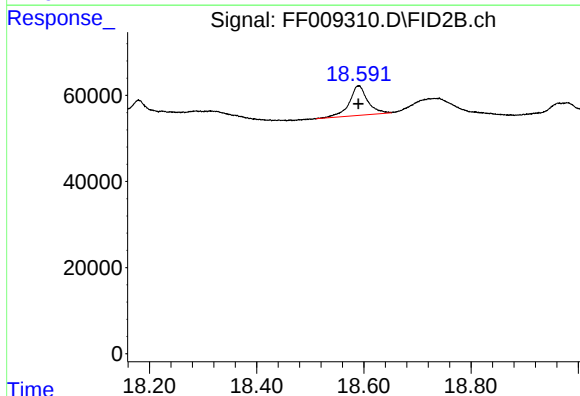


#14 N-DOTRIACONTANE

R.T.: 18.591 min
Delta R.T.: 0.001 min
Response: 162937
Conc: 1.52 ug/ml

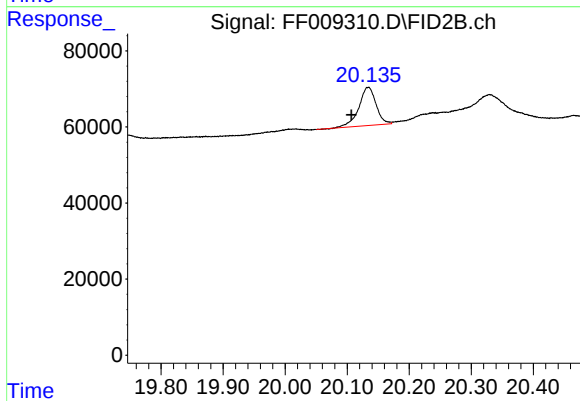

#16 N-HEXATRIACONTANE

R.T.: 20.135 min
Delta R.T.: 0.028 min
Response: 193994
Conc: 1.91 ug/ml

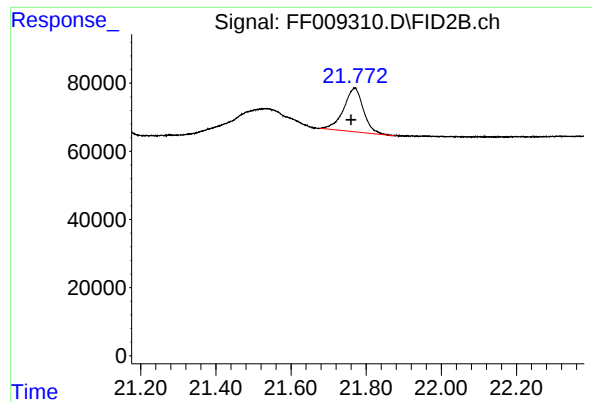

#18 N-TETRACONTANE

R.T.: 21.772 min
Delta R.T.: 0.012 min
Response: 468990
Conc: 4.86 ug/ml

Instrument :

FID_F

ClientSampleId :