

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
 Data File : FF009313.D
 Signal(s) : FID2B.ch
 Acq On : 09 Nov 2021 17:21
 Operator : AJ\MA
 Sample : M4507-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 10 00:57:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
 Quant Title :
 QLast Update : Tue Nov 09 14:23:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.704	2306810	20.619 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.593	54327	0.507 ug/ml
16) N-HEXATRIACONTANE	20.132	131728	1.295 ug/ml
18) N-TETRACONTANE	21.757	1314840	13.628 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009313.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 17:21
Operator : AJ\MA
Sample : M4507-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:57:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

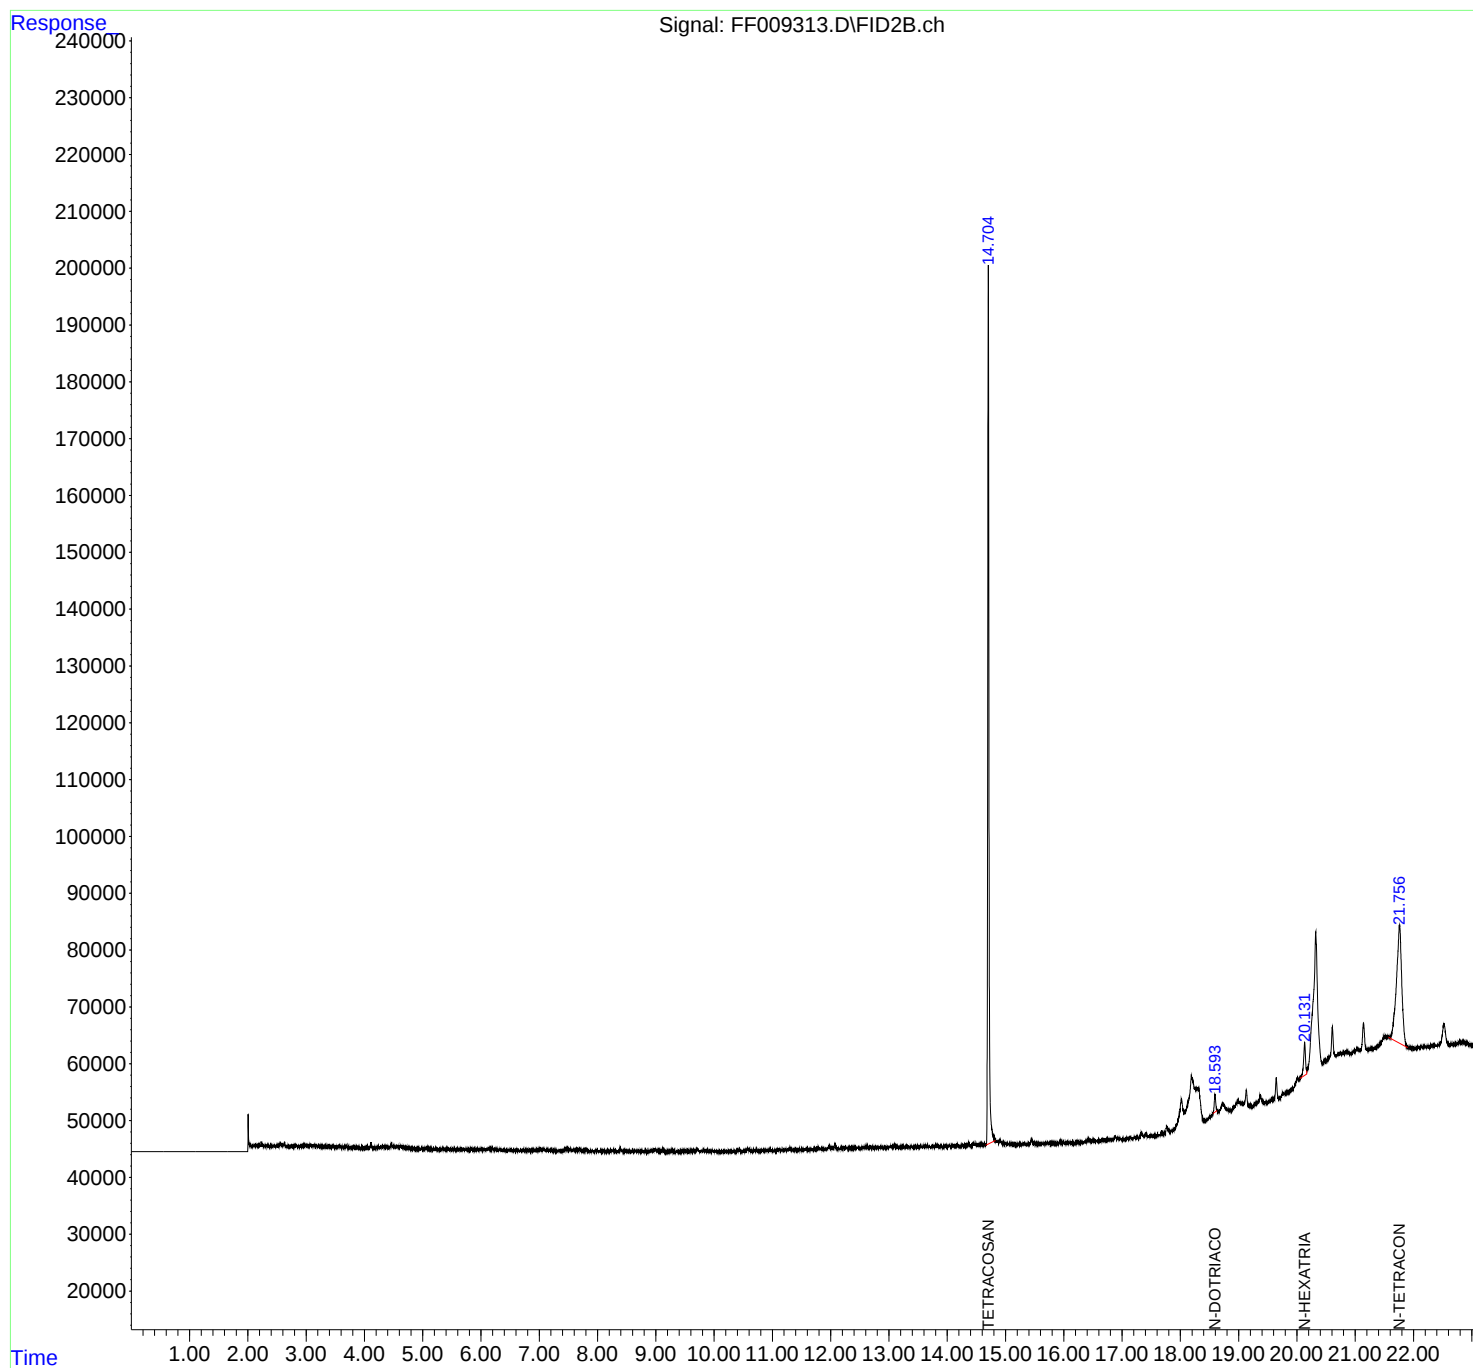


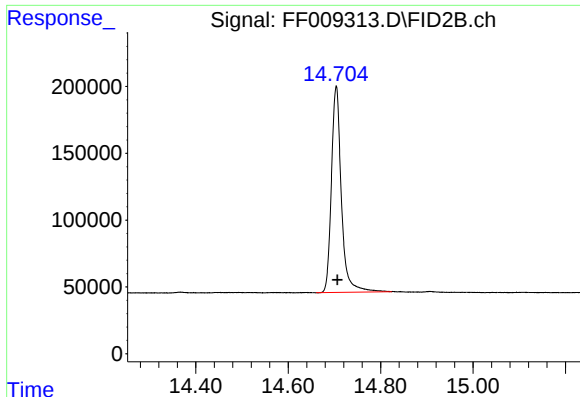

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.704 min
Delta R.T.: -0.002 min
Response: 2306810
Conc: 20.62 ug/ml

Instrument :
FID_F
ClientSampleId :

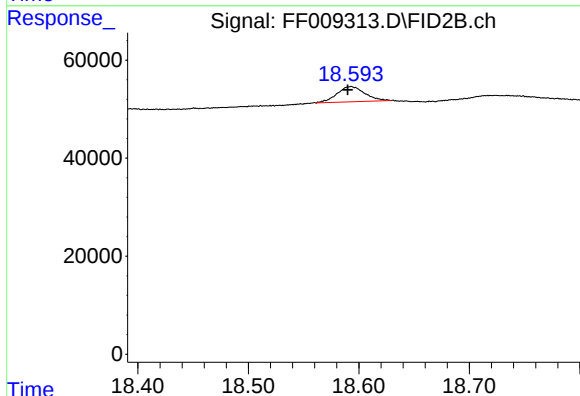


#14 N-DOTRIACONTANE

R.T.: 18.593 min
Delta R.T.: 0.003 min
Response: 54327
Conc: 0.51 ug/ml

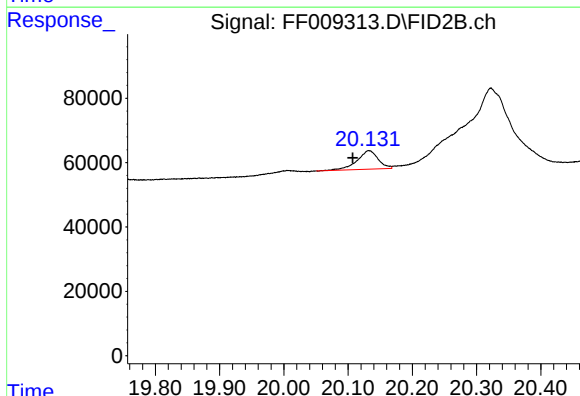

#16 N-HEXATRIACONTANE

R.T.: 20.132 min
Delta R.T.: 0.025 min
Response: 131728
Conc: 1.30 ug/ml

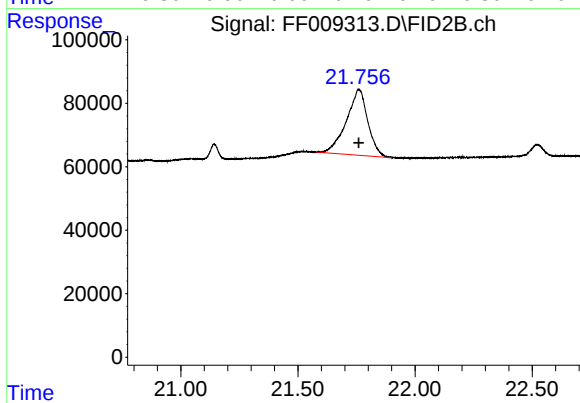

#18 N-TETRACONTANE

R.T.: 21.757 min
Delta R.T.: -0.003 min
Response: 1314840
Conc: 13.63 ug/ml