

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009314.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 17:52
Operator : AJ\MA
Sample : M4507-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:58:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.702	1902284	17.003 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.589	164863	1.539 ug/ml
16) N-HEXATRIACONTANE	20.130	201731	1.984 ug/ml
18) N-TETRACONTANE	21.768	354273	3.672 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009314.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 17:52
Operator : AJ\MA
Sample : M4507-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:58:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

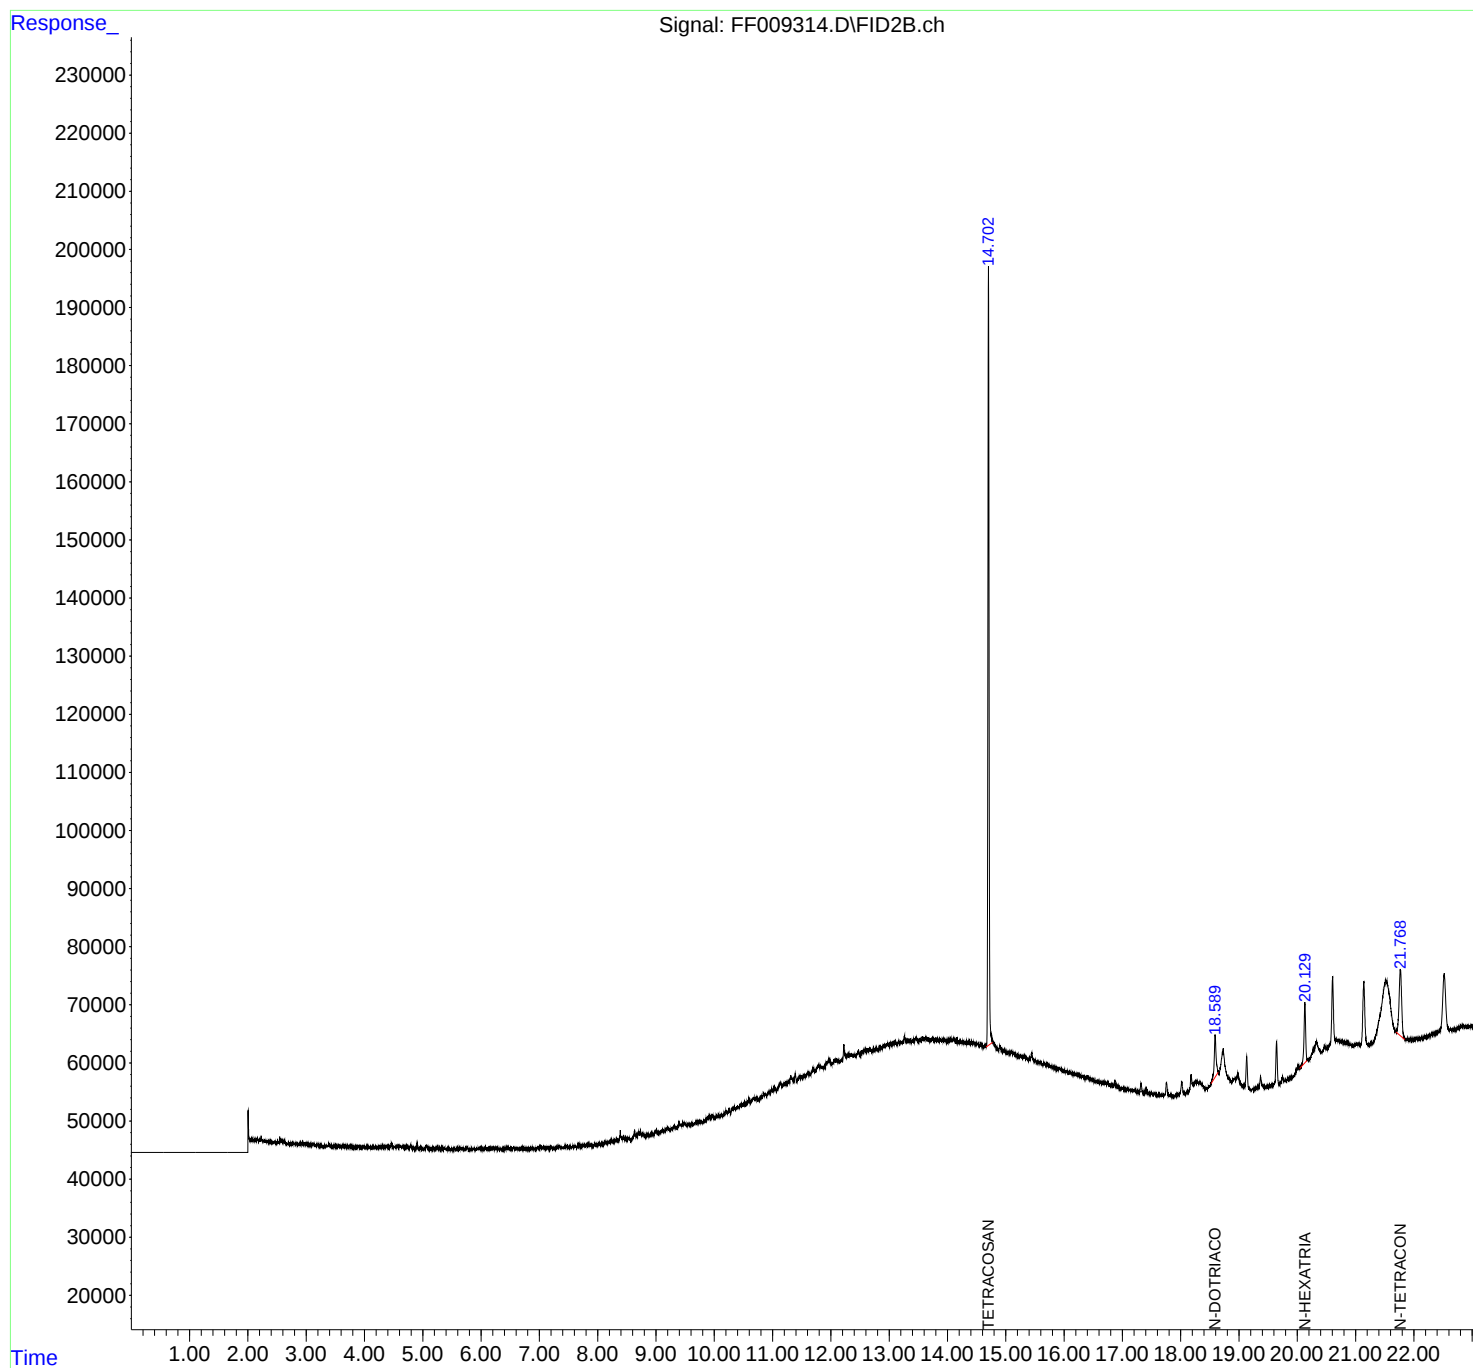


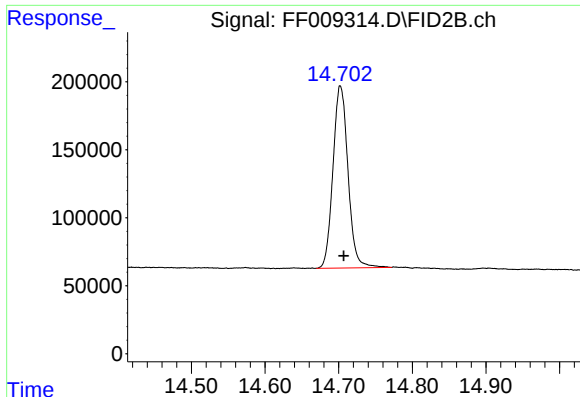

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.702 min
Delta R.T.: -0.005 min
Response: 1902284
Conc: 17.00 ug/ml

Instrument :
FID_F
ClientSampleId :

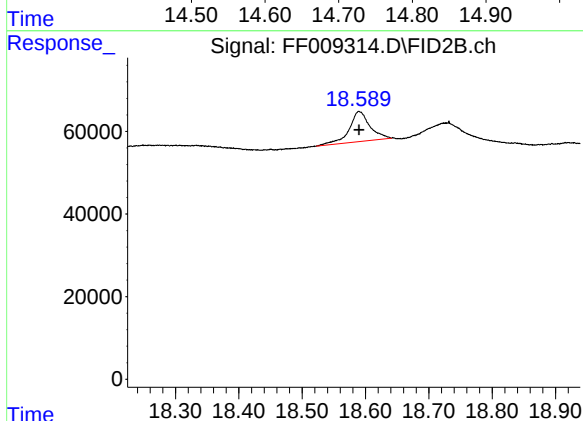


#14 N-DOTRIACONTANE

R.T.: 18.589 min
Delta R.T.: 0.000 min
Response: 164863
Conc: 1.54 ug/ml

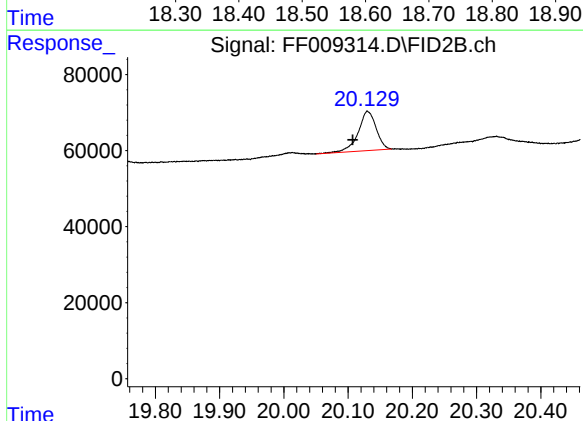

#16 N-HEXATRIACONTANE

R.T.: 20.130 min
Delta R.T.: 0.023 min
Response: 201731
Conc: 1.98 ug/ml

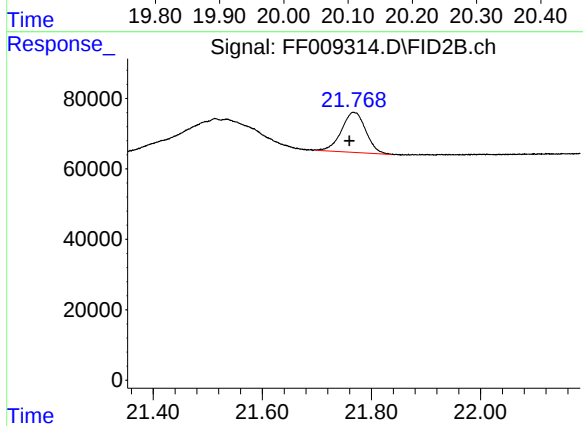

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: 0.008 min
Response: 354273
Conc: 3.67 ug/ml