

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009317.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 19:25
Operator : AJ\MA
Sample : M4507-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:59:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.701	2000080	17.877 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.590	125916	1.176 ug/ml
16) N-HEXATRIACONTANE	20.132	533257	5.244 ug/ml
18) N-TETRACONTANE	21.771	696363	7.218 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009317.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 19:25
Operator : AJ\MA
Sample : M4507-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:59:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

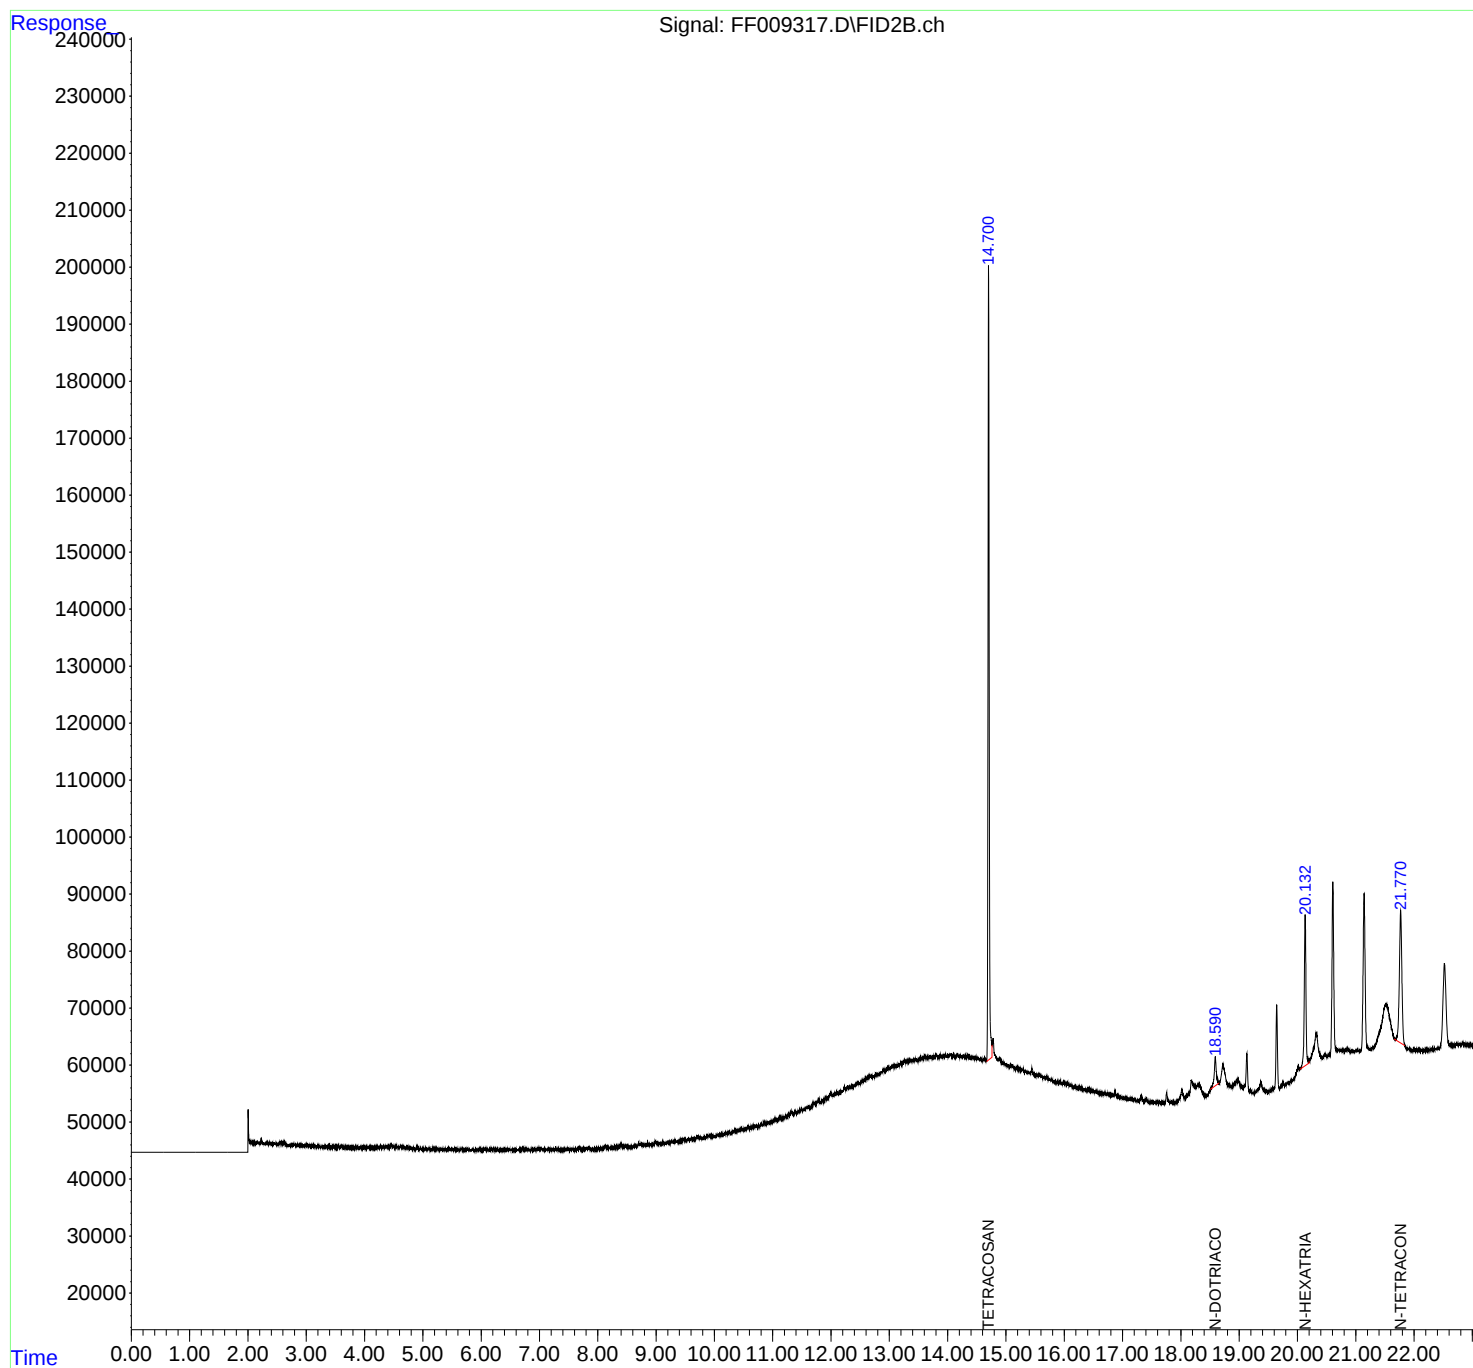


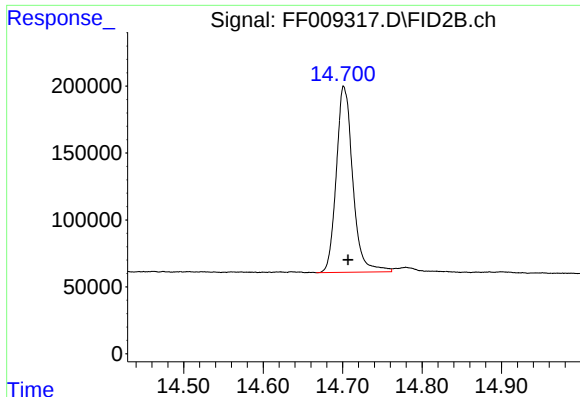

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.701 min
Delta R.T.: -0.006 min
Response: 2000080
Conc: 17.88 ug/ml

Instrument :
FID_F
ClientSampleId :

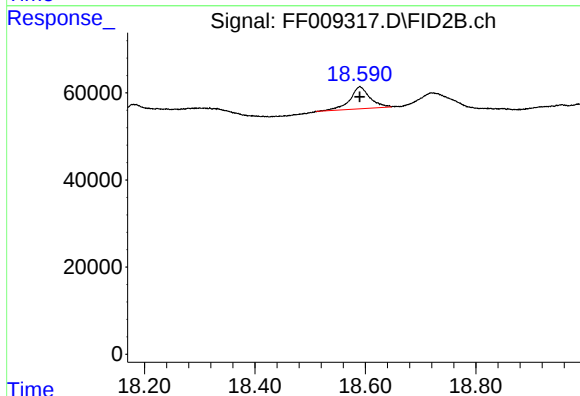


#14 N-DOTRIACONTANE

R.T.: 18.590 min
Delta R.T.: 0.000 min
Response: 125916
Conc: 1.18 ug/ml

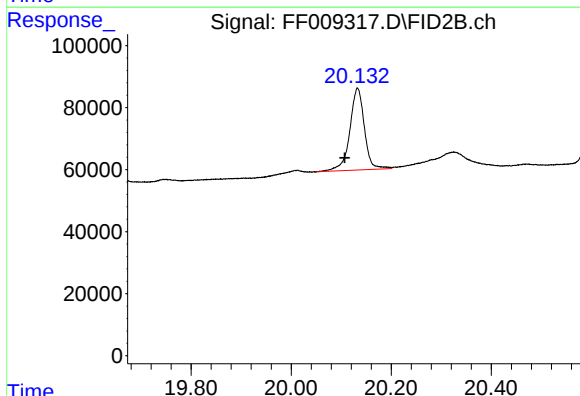

#16 N-HEXATRIACONTANE

R.T.: 20.132 min
Delta R.T.: 0.025 min
Response: 533257
Conc: 5.24 ug/ml

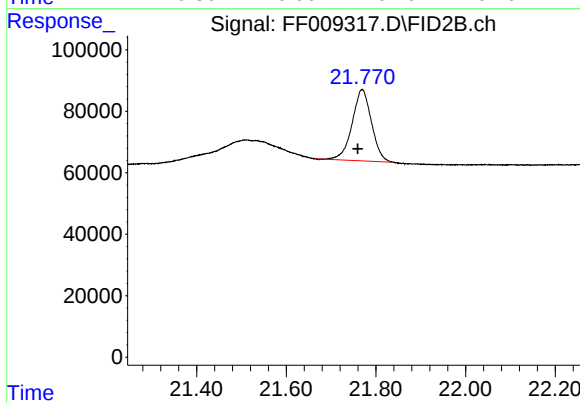

#18 N-TETRACONTANE

R.T.: 21.771 min
Delta R.T.: 0.011 min
Response: 696363
Conc: 7.22 ug/ml