

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009319.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 20:27
Operator : AJ\MA
Sample : M4507-10
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:59:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.701	1899925	16.982 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.589	74647	0.697 ug/ml
16) N-HEXATRIACONTANE	20.132	338550	3.329 ug/ml
18) N-TETRACONTANE	21.770	1075302	11.145 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009319.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 20:27
Operator : AJ\MA
Sample : M4507-10
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:59:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

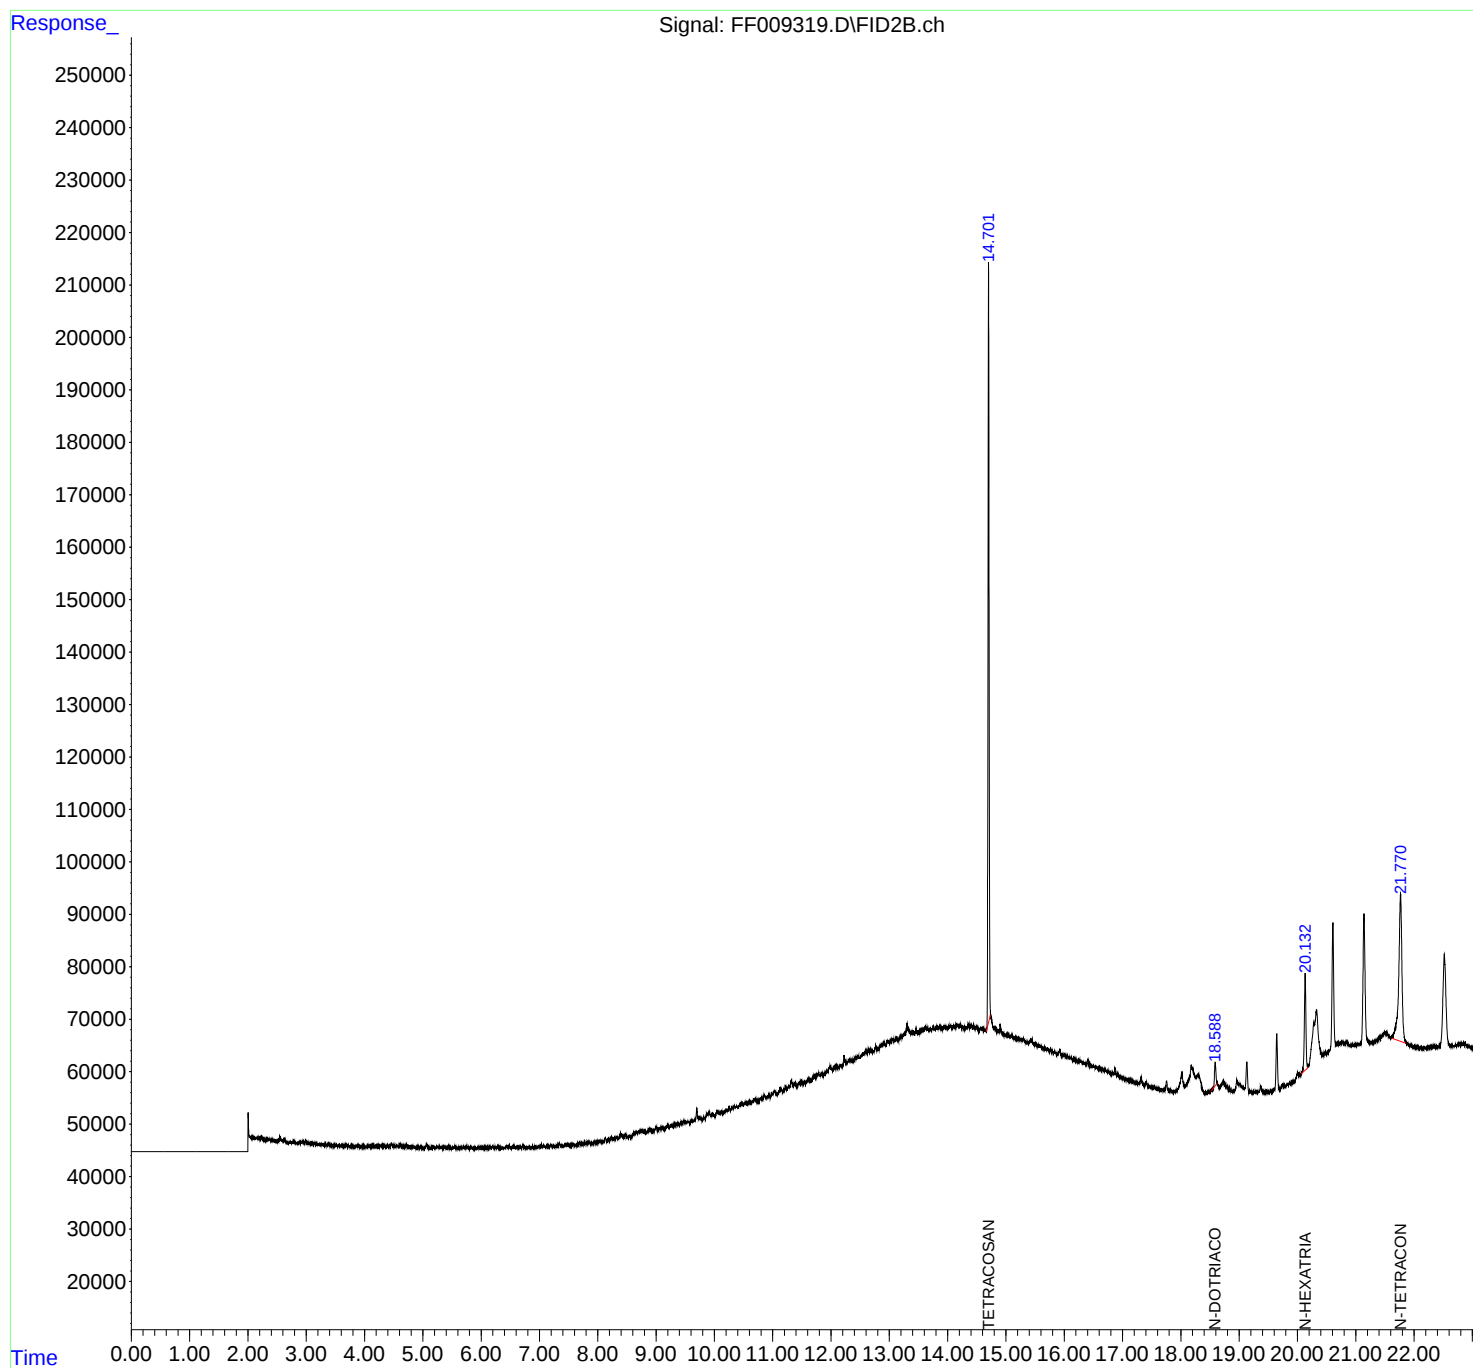


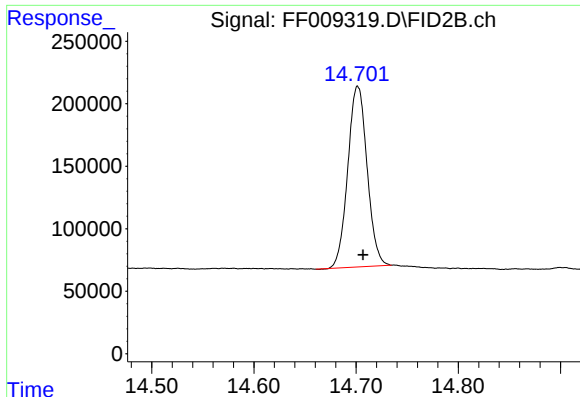

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.701 min
Delta R.T.: -0.005 min
Response: 1899925
Conc: 16.98 ug/ml

Instrument :
FID_F
ClientSampleId :

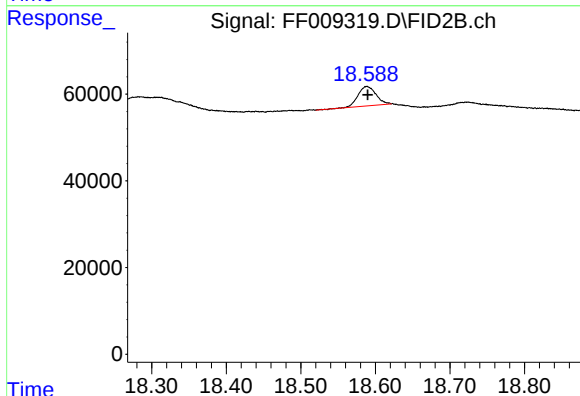


#14 N-DOTRIACONTANE

R.T.: 18.589 min
Delta R.T.: -0.001 min
Response: 74647
Conc: 0.70 ug/ml

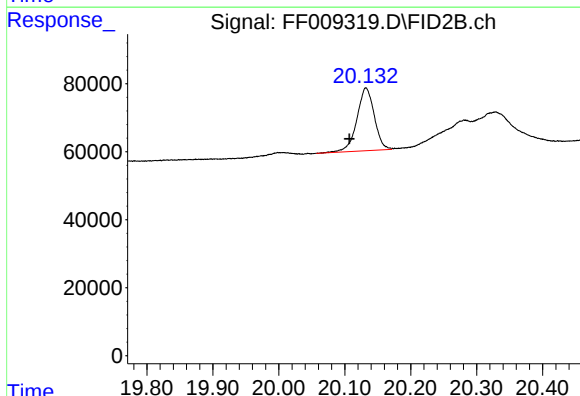

#16 N-HEXATRIACONTANE

R.T.: 20.132 min
Delta R.T.: 0.025 min
Response: 338550
Conc: 3.33 ug/ml

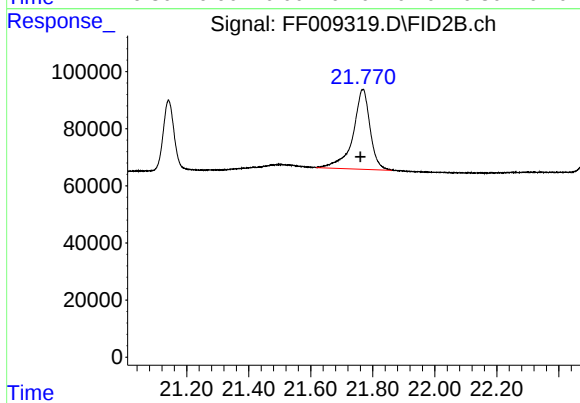

#18 N-TETRACONTANE

R.T.: 21.770 min
Delta R.T.: 0.010 min
Response: 1075302
Conc: 11.15 ug/ml