

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009320.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 20:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 01:00:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.704	2244477	20.061 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.594	87361	0.816 ug/ml
16) N-HEXATRIACONTANE	20.132	143203	1.408 ug/ml
18) N-TETRACONTANE	21.767	641773	6.652 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009320.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 20:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 01:00:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

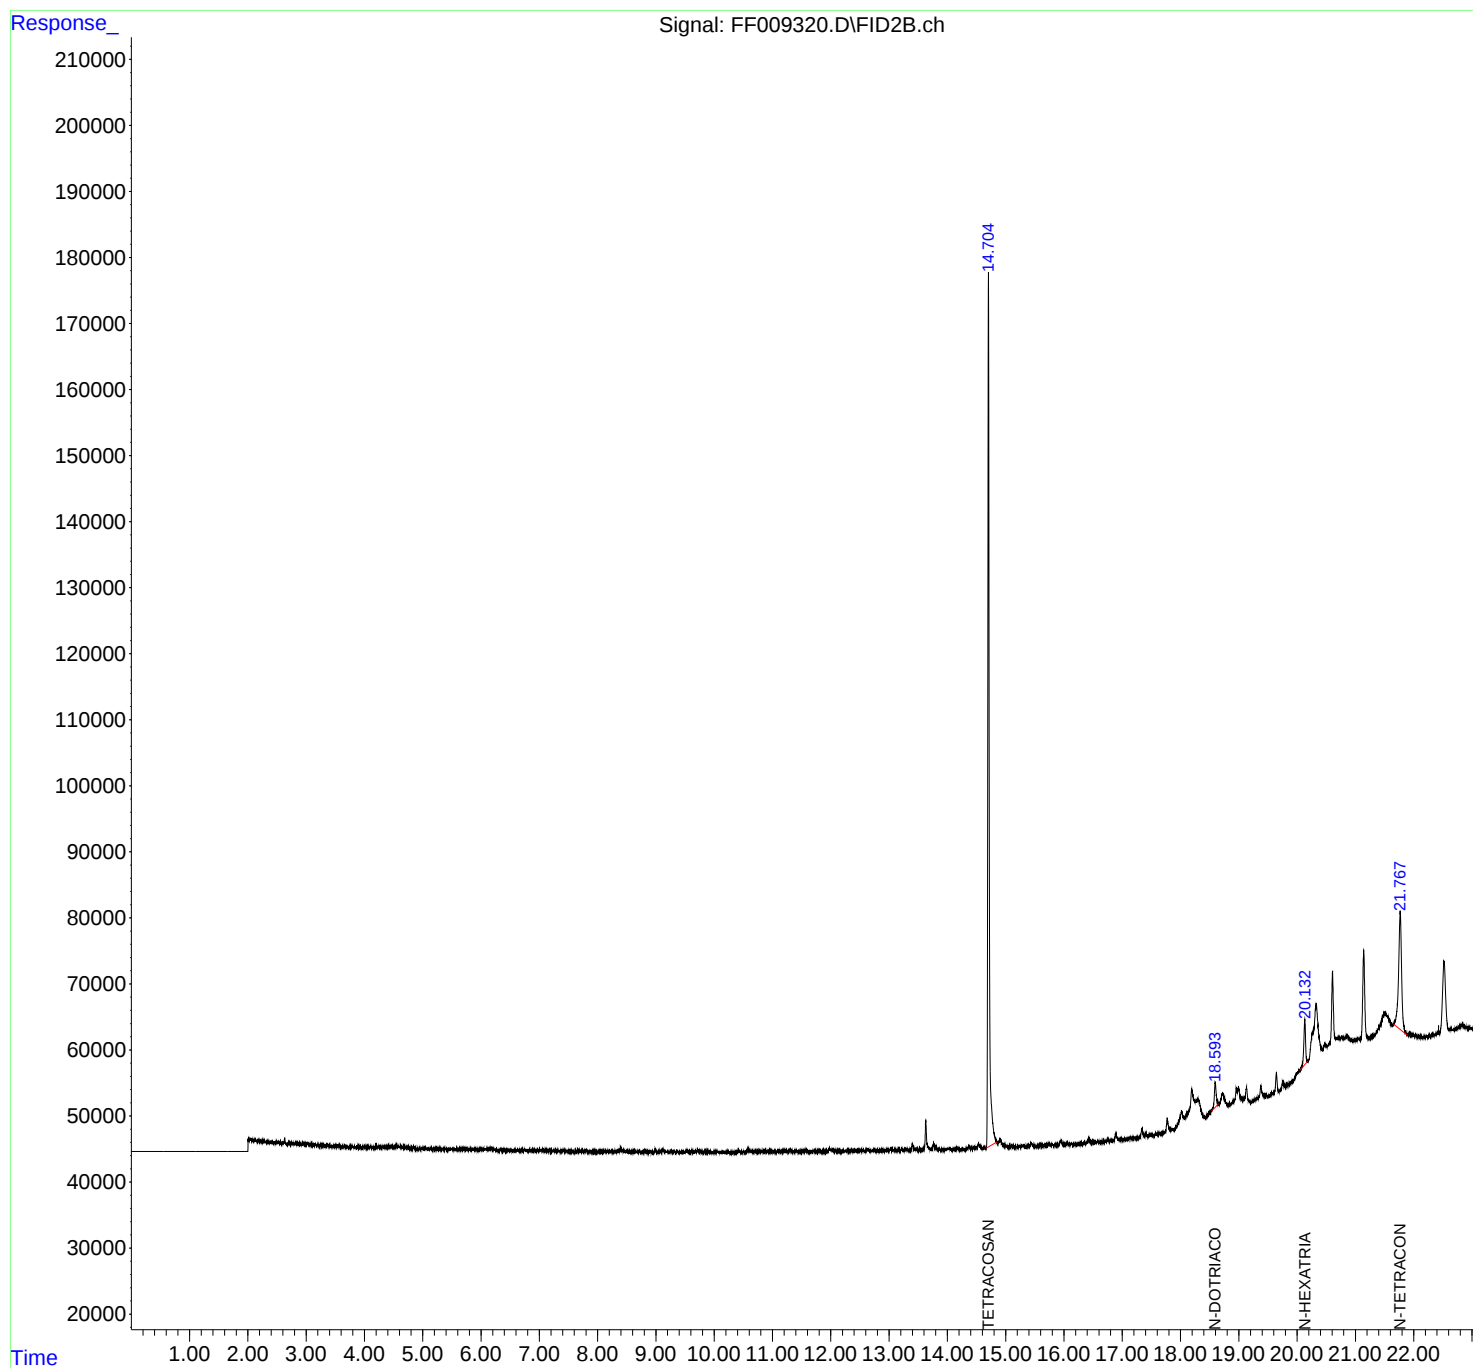


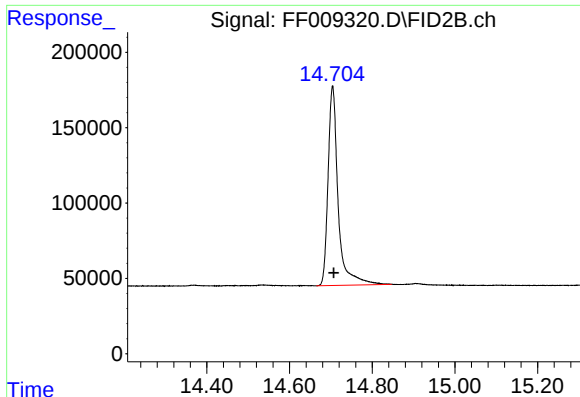

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.704 min
Delta R.T.: -0.003 min
Response: 2244477
Conc: 20.06 ug/ml

Instrument :
FID_F
ClientSampleId :

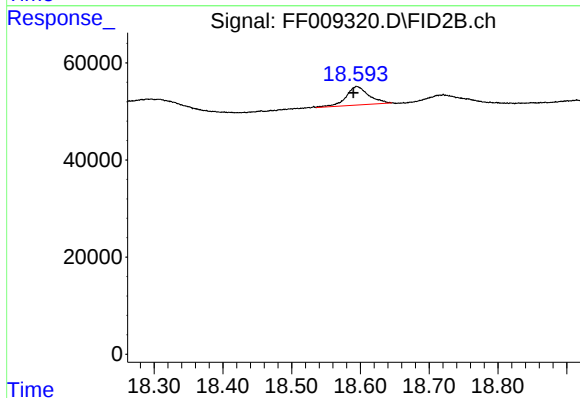


#14 N-DOTRIACONTANE

R.T.: 18.594 min
Delta R.T.: 0.004 min
Response: 87361
Conc: 0.82 ug/ml

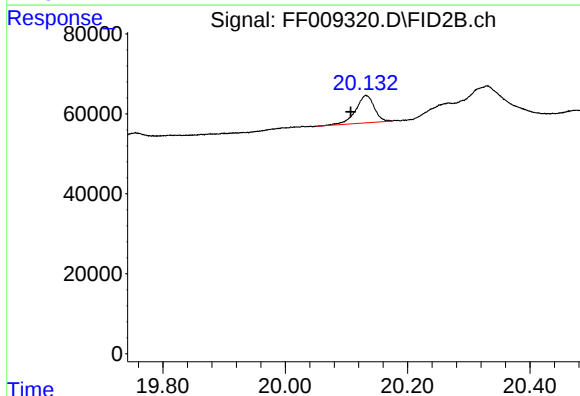

#16 N-HEXATRIACONTANE

R.T.: 20.132 min
Delta R.T.: 0.025 min
Response: 143203
Conc: 1.41 ug/ml

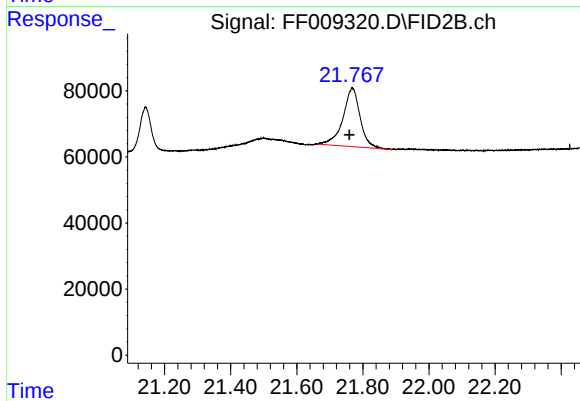

#18 N-TETRACONTANE

R.T.: 21.767 min
Delta R.T.: 0.007 min
Response: 641773
Conc: 6.65 ug/ml