

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009309.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 15:17
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 10 00:56:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.477	5250907	37.557 ug/ml
12) N-OCTACOSANE	16.874	5012517	42.844 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009309.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 15:17
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 10 00:56:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

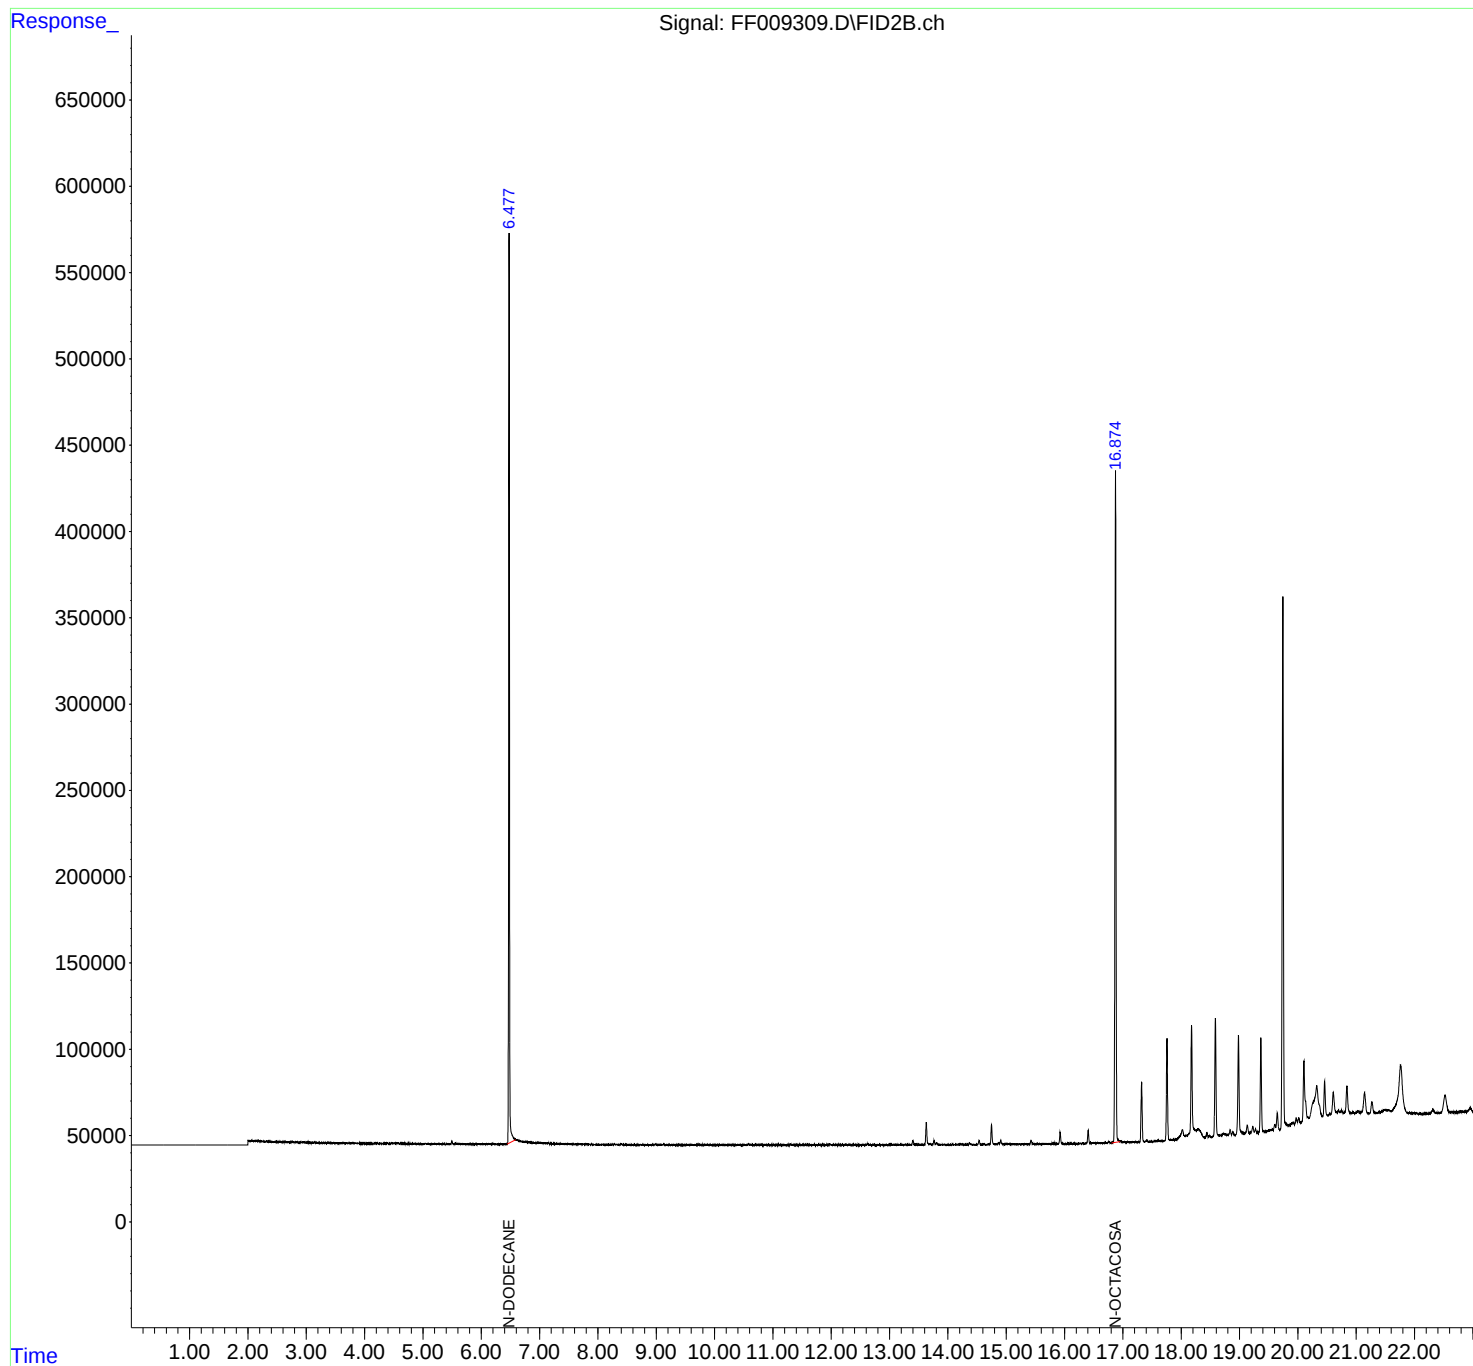


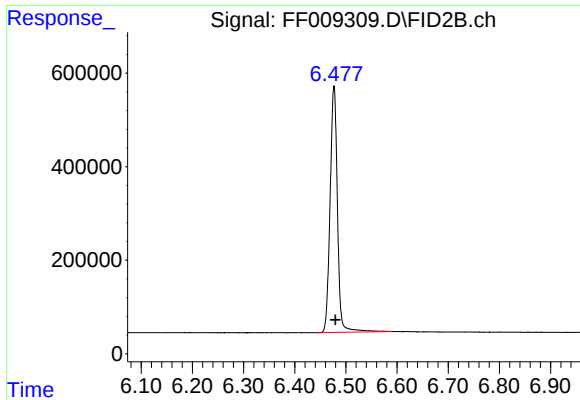

#3 N-DODECANE


R.T.: 6.477 min
Delta R.T.: -0.002 min
Response: 5250907
Conc: 37.56 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

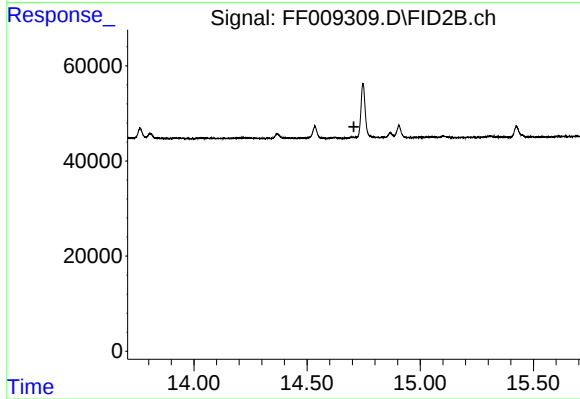

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.707 min
Response: 0
Conc: N.D.

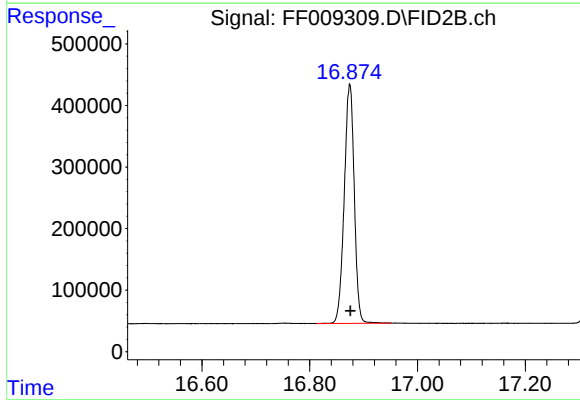

#12 N-OCTACOSANE

R.T.: 16.874 min
Delta R.T.: 0.000 min
Response: 5012517
Conc: 42.84 ug/ml