

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009318.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 19:56
Operator : AJ\MA
Sample : M4507-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
BW-15-20211103-A

Integration File: autoint1.e
Quant Time: Nov 10 00:59:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.704	2044277	18.272 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110921\
Data File : FF009318.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2021 19:56
Operator : AJ\MA
Sample : M4507-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
BW-15-20211103-A

Integration File: autoint1.e
Quant Time: Nov 10 00:59:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110921.M
Quant Title :
QLast Update : Tue Nov 09 14:23:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

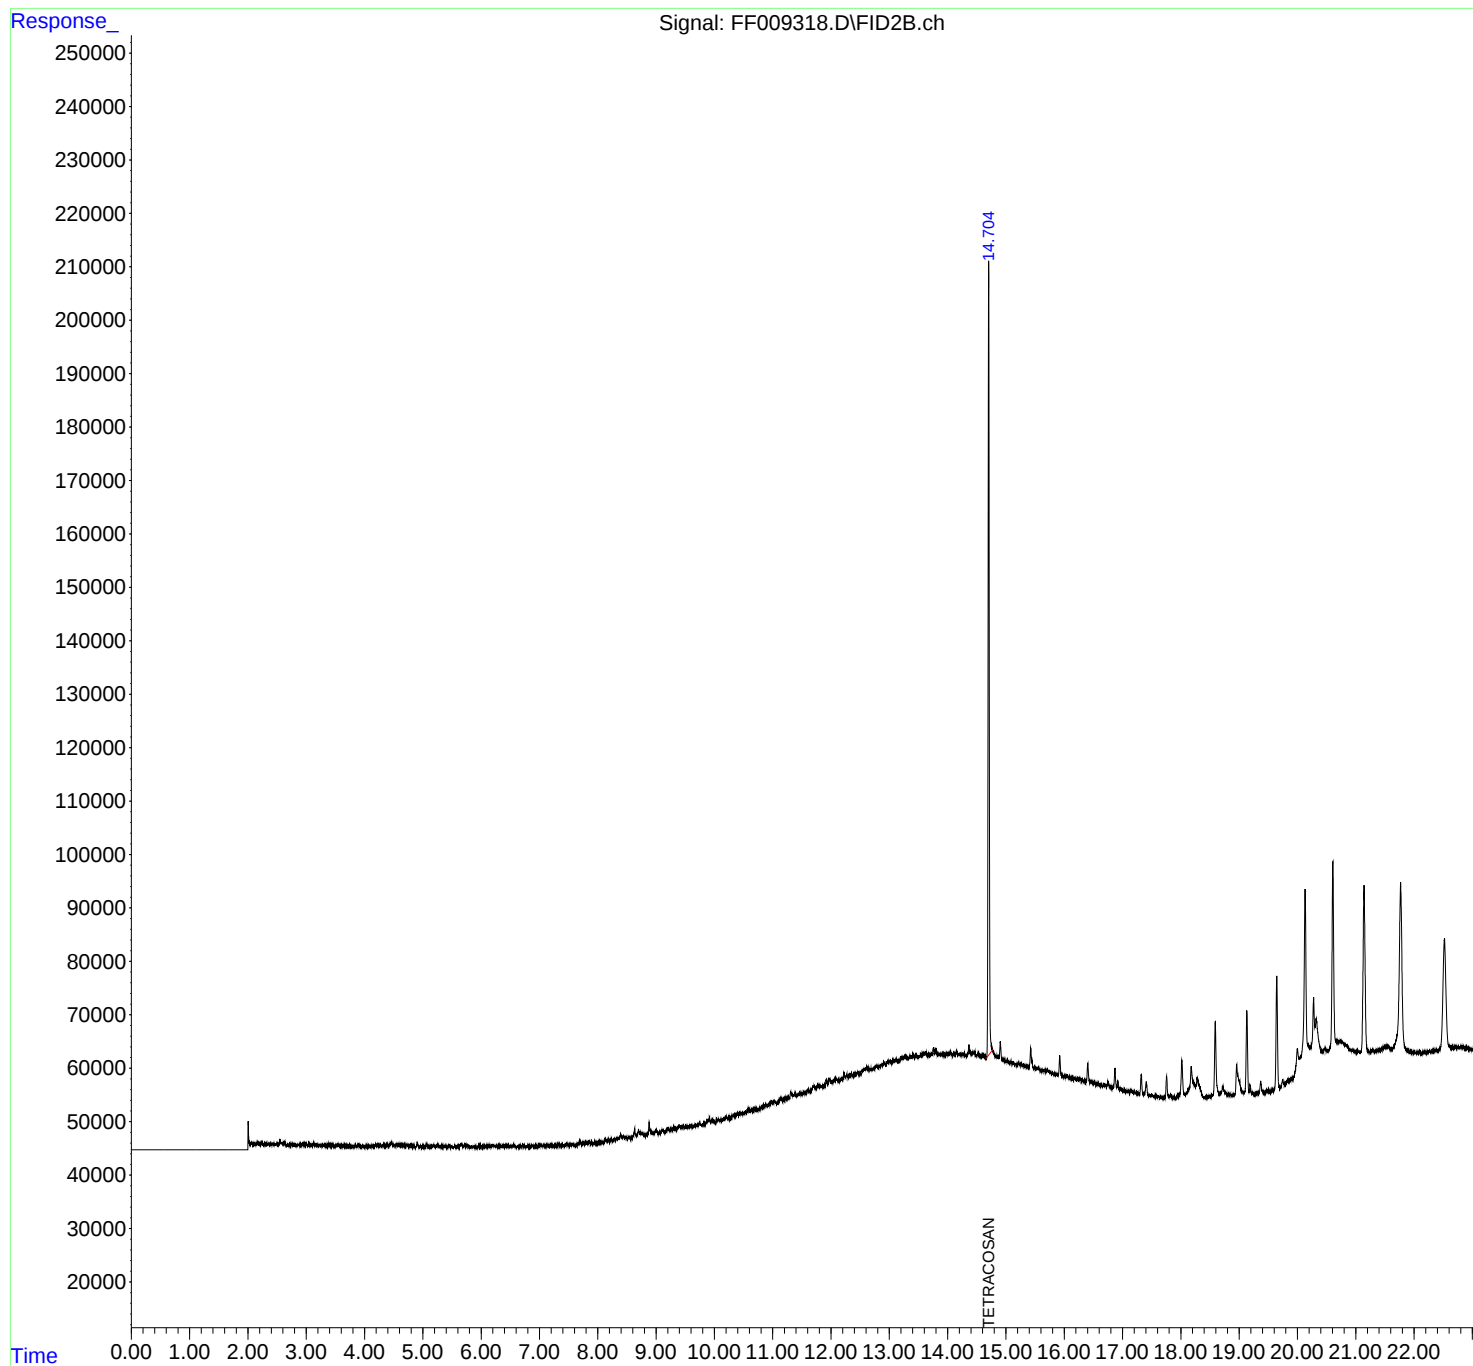

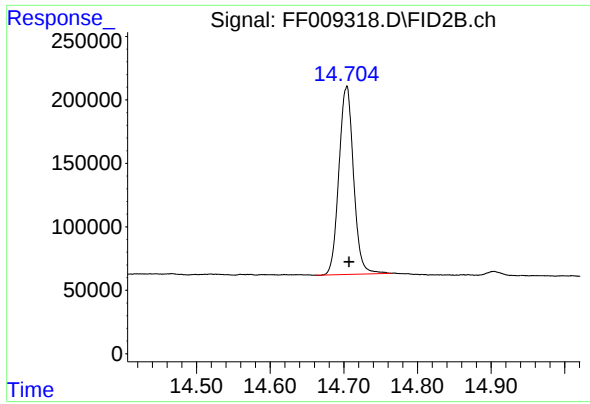

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.704 min
Delta R.T.: -0.002 min
Response: 2044277
Conc: 18.27 ug/ml

Instrument :

FID_F

ClientSampleId :

BW-15-20211103-A