

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110922\
 Data File : FF011599.D
 Signal(s) : FID2B.ch
 Acq On : 09 Nov 2022 20:35
 Operator : YP\AJ
 Sample : PB148882BS
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB148882BS

Integration File: autoint1.e
 Quant Time: Nov 10 03:57:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	1841113	15.518 ug/ml
Target Compounds			
2) N-DECANE	4.616	2162157	16.382 ug/ml
3) N-DODECANE	6.776	2195093	16.332 ug/ml
4) N-TETRADECANE	8.601	2198146	16.243 ug/ml
5) N-HEXADECANE	10.207	2222892	16.169 ug/ml
6) N-OCTADECANE	11.648	2223704	16.076 ug/ml
7) N-EICOSANE	12.958	2186178	15.808 ug/ml
8) N-DOCOSANE	14.156	2101963	15.573 ug/ml
10) N-TETRACOSANE	15.259	2081944	15.352 ug/ml
11) N-HEXACOSANE	16.280	2024713	15.154 ug/ml
12) N-OCTACOSANE	17.230	1992667	15.041 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110922\
Data File : FF011599.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2022 20:35
Operator : YP\AJ
Sample : PB148882BS
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB148882BS

Integration File: autoint1.e
Quant Time: Nov 10 03:57:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

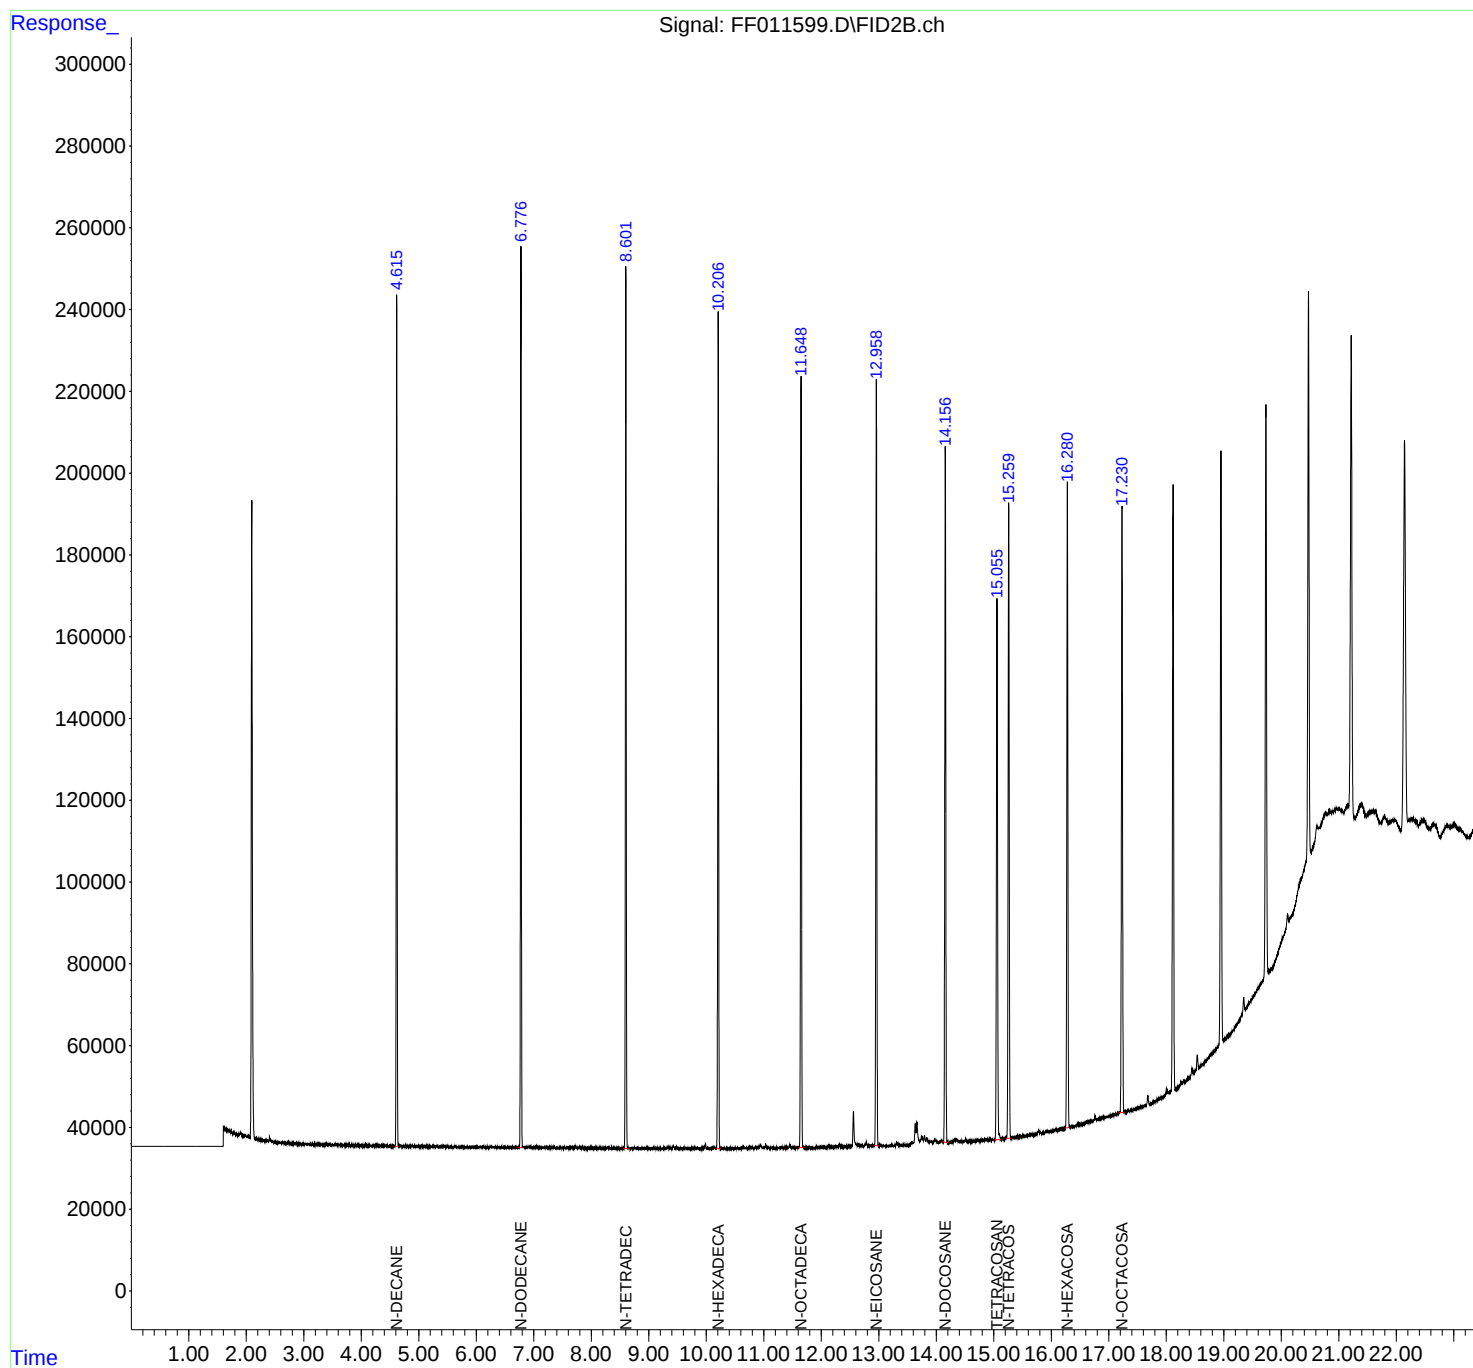


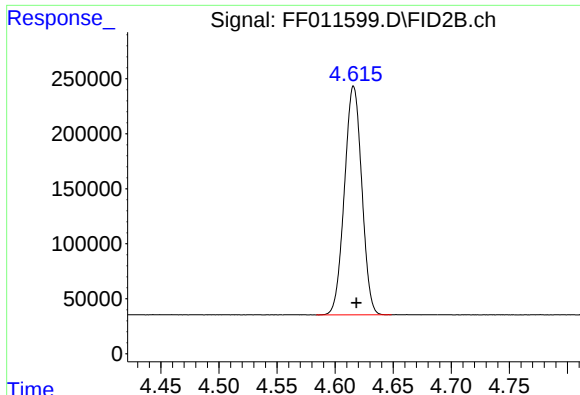

#2 N-DECANE


R.T.: 4.616 min
Delta R.T.: -0.002 min
Response: 2162157
Conc: 16.38 ug/ml

Instrument :
FID_F
ClientSampleId :
PB148882BS

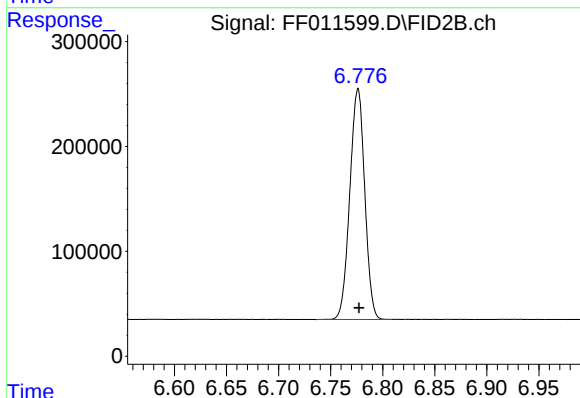


#3 N-DODECANE

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 2195093
Conc: 16.33 ug/ml

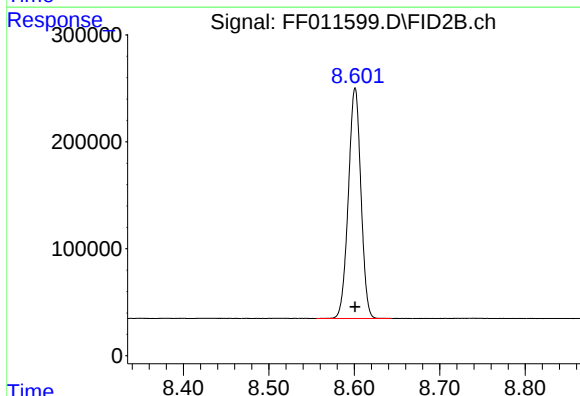


#4 N-TETRADECANE

R.T.: 8.601 min
Delta R.T.: 0.000 min
Response: 2198146
Conc: 16.24 ug/ml

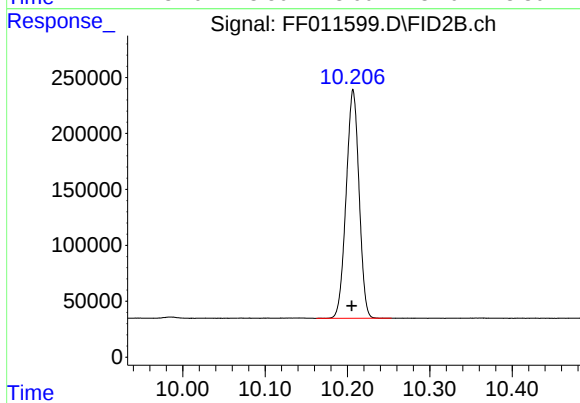

#5 N-HEXADECANE


R.T.: 10.207 min
Delta R.T.: 0.002 min
Response: 2222892
Conc: 16.17 ug/ml

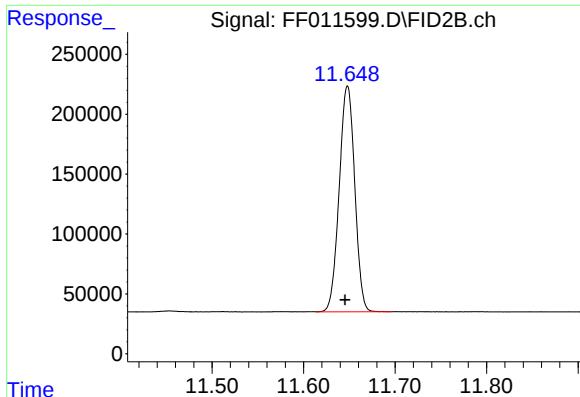

#6 N-OCTADECANE


R.T.: 11.648 min
Delta R.T.: 0.003 min
Response: 2223704
Conc: 16.08 ug/ml

Instrument :
FID_F
ClientSampleId :
PB148882BS

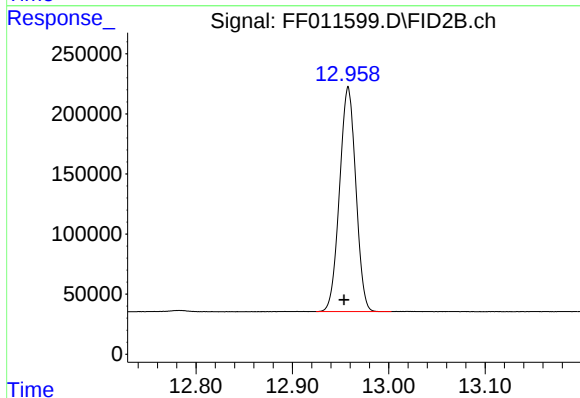


#7 N-EICOSANE

R.T.: 12.958 min
Delta R.T.: 0.005 min
Response: 2186178
Conc: 15.81 ug/ml

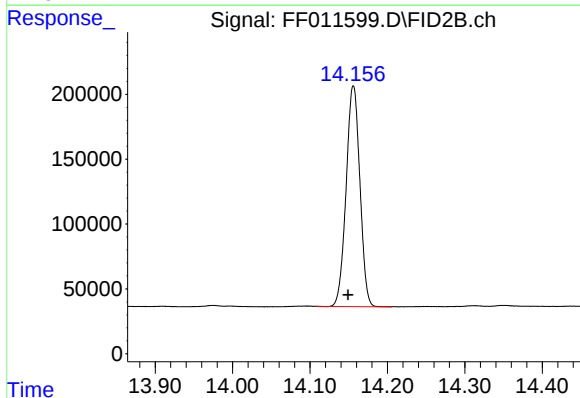


#8 N-DOCOSANE

R.T.: 14.156 min
Delta R.T.: 0.007 min
Response: 2101963
Conc: 15.57 ug/ml

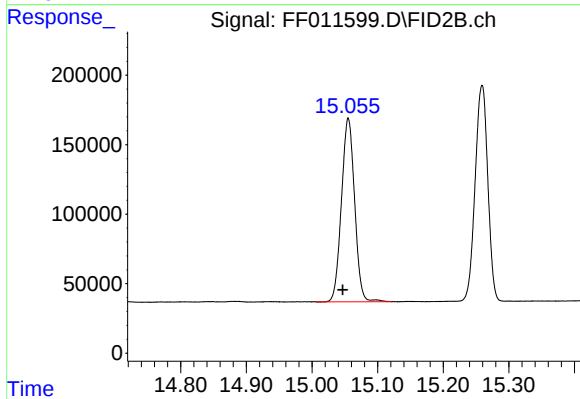

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.055 min
Delta R.T.: 0.008 min
Response: 1841113
Conc: 15.52 ug/ml

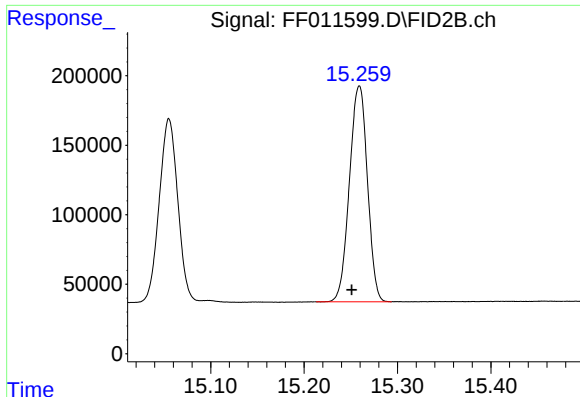

#10 N-TETRACOSANE


R.T.: 15.259 min
Delta R.T.: 0.008 min
Response: 2081944
Conc: 15.35 ug/ml

Instrument :
FID_F
ClientSampleId :
PB148882BS

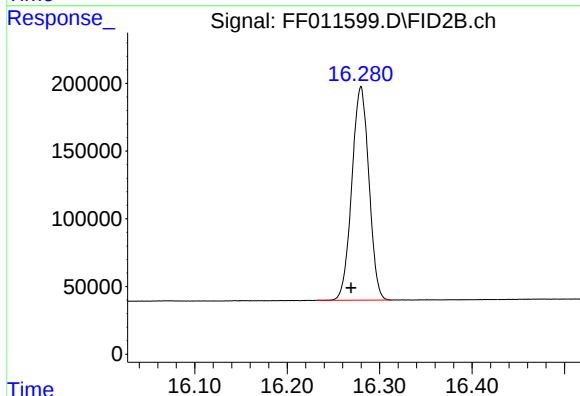

#11 N-HEXACOSANE

R.T.: 16.280 min
Delta R.T.: 0.011 min
Response: 2024713
Conc: 15.15 ug/ml

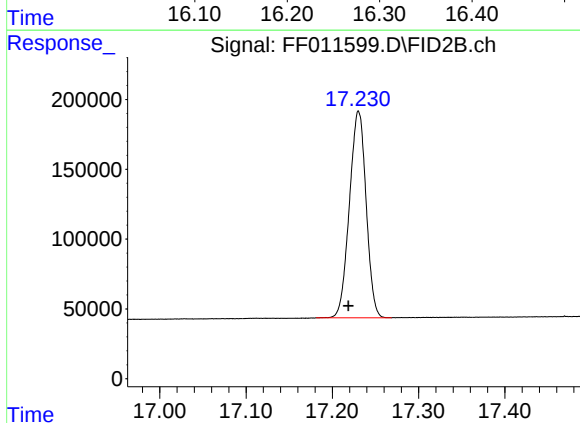

#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: 0.012 min
Response: 1992667
Conc: 15.04 ug/ml