

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111018\
 Data File : FF002638.D
 Signal(s) : FID2B.ch
 Acq On : 09 Nov 2018 14:48
 Operator : AJ\SJ
 Sample : J5269-04 MS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 21:02:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.634	2062564	14.839 ug/ml
Target Compounds			
2) N-DECANE	4.372	1751886	11.469 ug/ml
3) N-DODECANE	6.392	2005917	12.954 ug/ml
4) N-TETRADECANE	8.184	2167764	13.853 ug/ml
5) N-HEXADECANE	9.784	2234257	14.216 ug/ml
6) N-OCTADECANE	11.226	2220426	13.972 ug/ml
7) N-EICOSANE	12.536	2212201	13.967 ug/ml
8) N-DOCOSANE	13.734	2203274	13.966 ug/mlm
10) N-TETRACOSANE	14.838	2123873	13.575 ug/ml
11) N-HEXACOSANE	15.859	2144023	13.769 ug/ml
12) N-OCTACOSANE	16.810	2336401	15.062 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111018\
Data File : FF002638.D
Signal(s) : FID2B.ch
Acq On : 09 Nov 2018 14:48
Operator : AJ\SJ
Sample : J5269-04 MS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 21:02:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

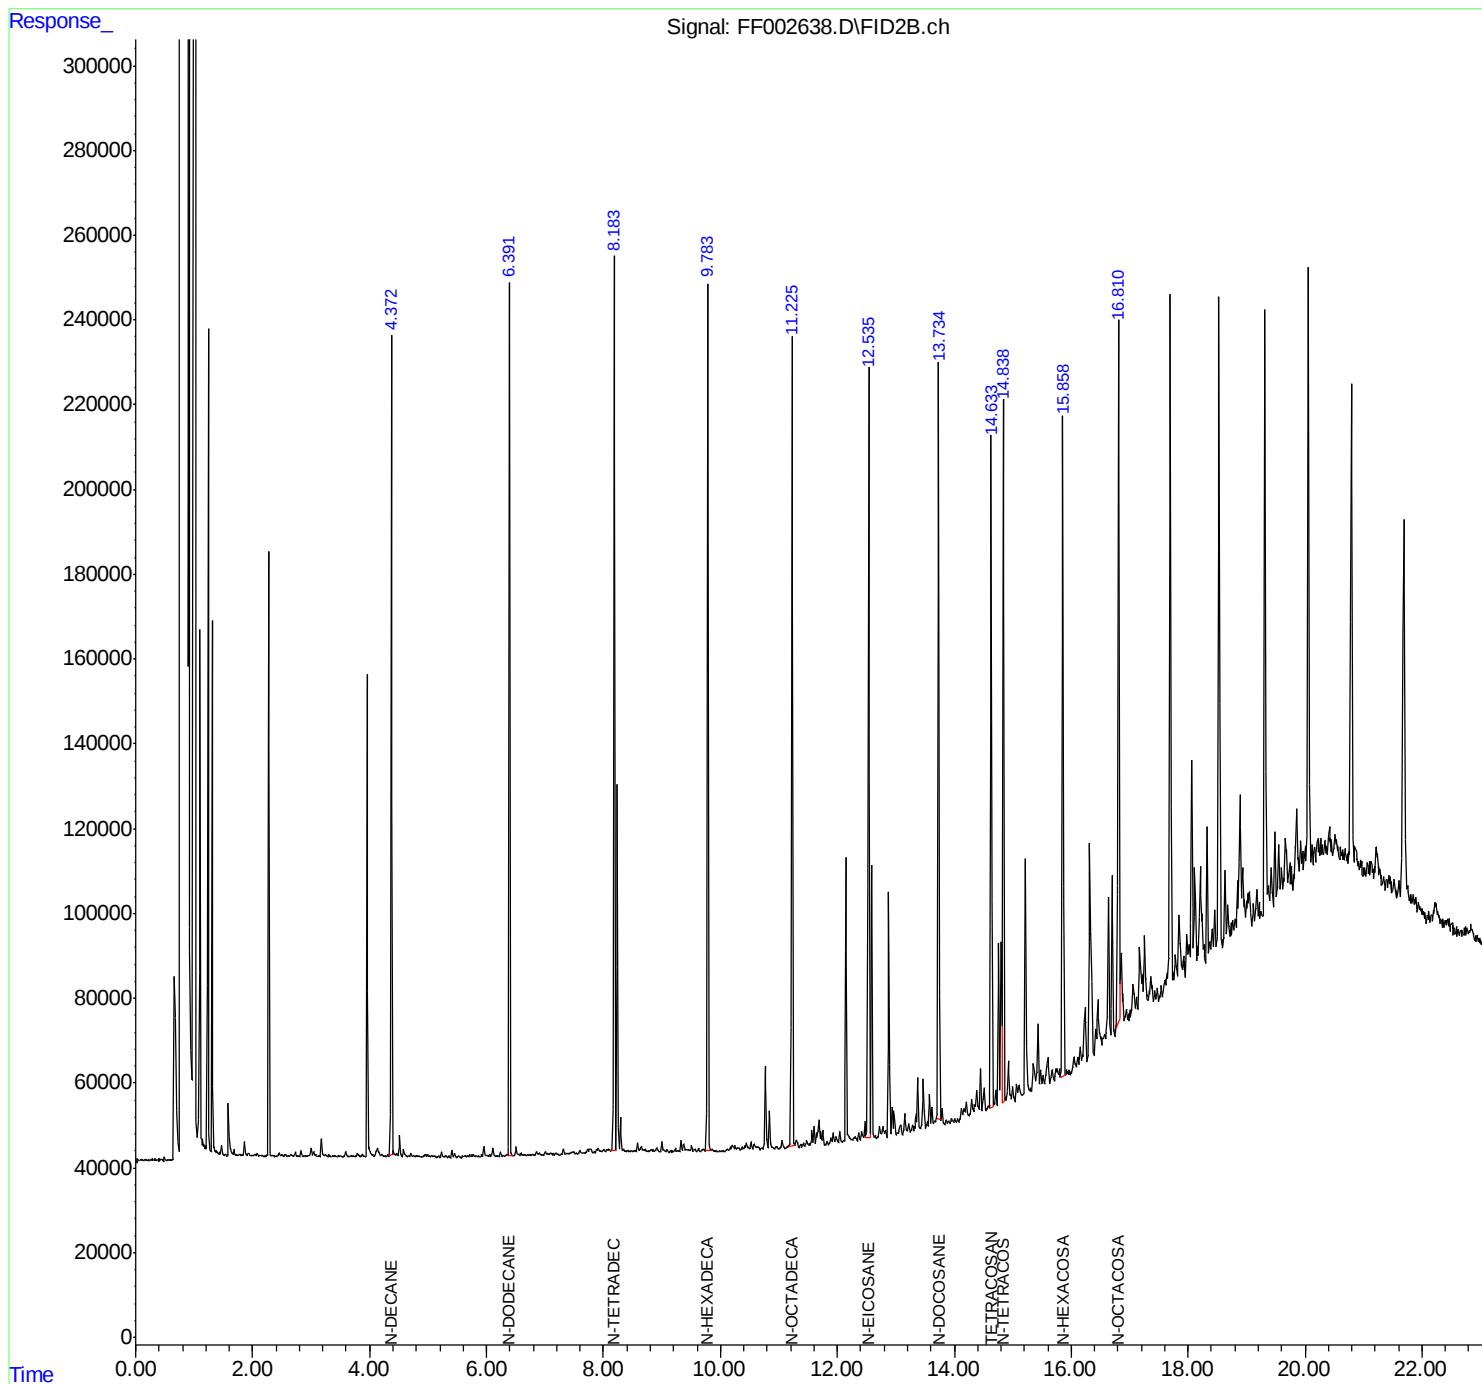

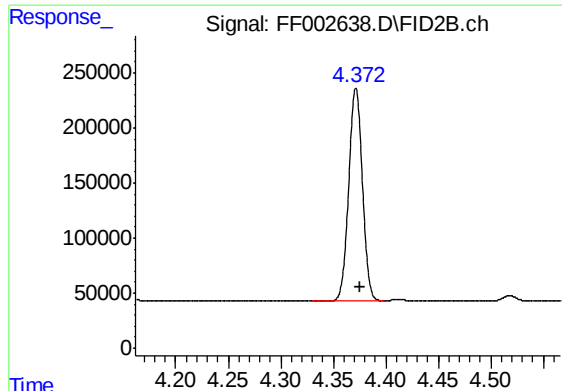


#2 N-DECANE

R.T.: 4.372 min
Delta R.T.: -0.004 min
Response: 1751886
Conc: 11.47 ug/ml

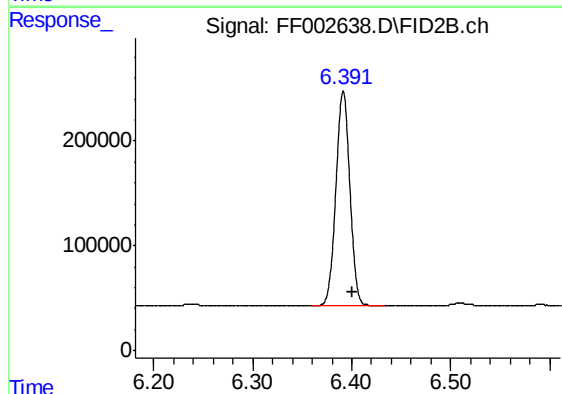


#3 N-DODECANE

R.T.: 6.392 min
Delta R.T.: -0.009 min
Response: 2005917
Conc: 12.95 ug/ml

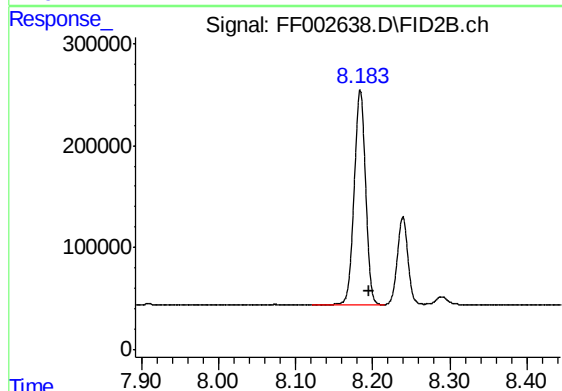


#4 N-TETRADECANE

R.T.: 8.184 min
Delta R.T.: -0.012 min
Response: 2167764
Conc: 13.85 ug/ml

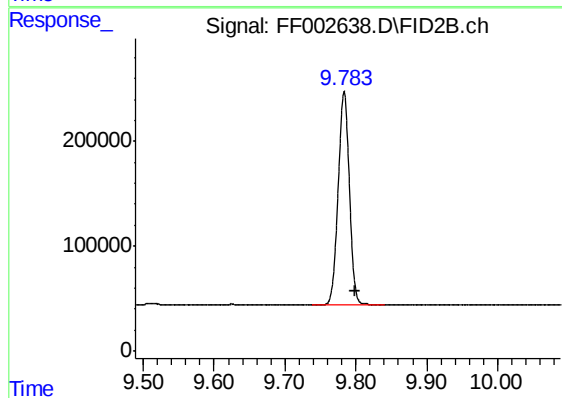


#5 N-HEXADECANE

R.T.: 9.784 min
Delta R.T.: -0.015 min
Response: 2234257
Conc: 14.22 ug/ml

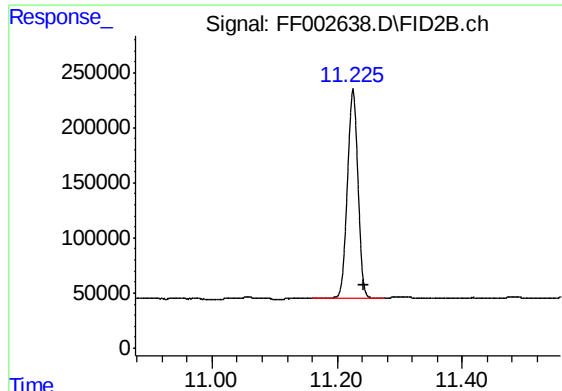


#6 N-OCTADECANE

R.T.: 11.226 min
Delta R.T.: -0.017 min
Response: 2220426
Conc: 13.97 ug/ml

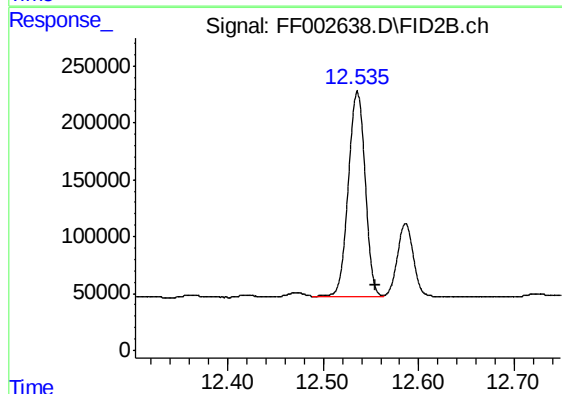


#7 N-EICOSANE

R.T.: 12.536 min
Delta R.T.: -0.019 min
Response: 2212201
Conc: 13.97 ug/ml

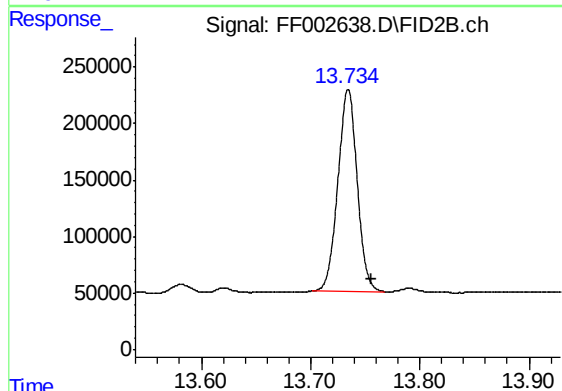


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: -0.022 min
Response: 2203274
Conc: 13.97 ug/ml m

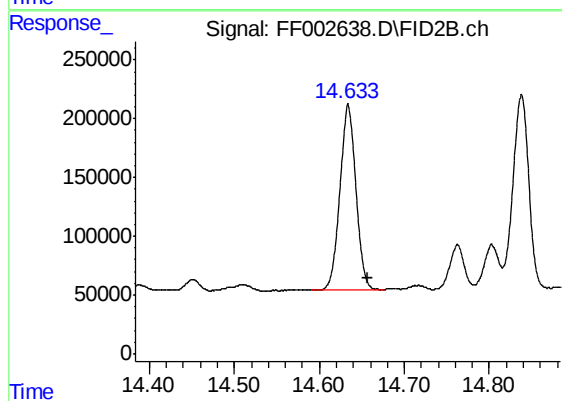


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.634 min
Delta R.T.: -0.022 min
Response: 2062564
Conc: 14.84 ug/ml

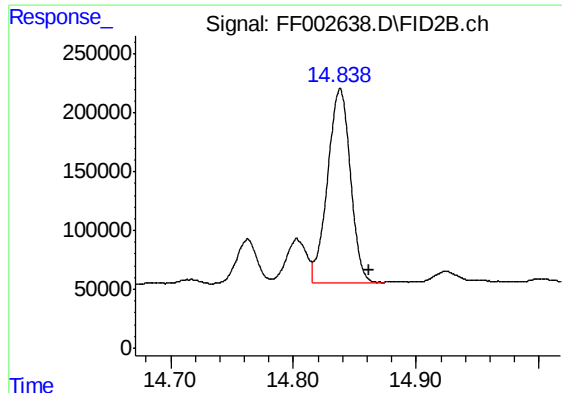


#10 N-TETRACOSANE

R.T.: 14.838 min
Delta R.T.: -0.024 min
Response: 2123873
Conc: 13.58 ug/ml

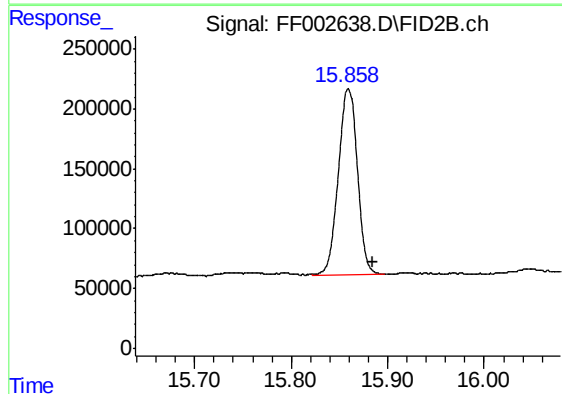

#11 N-HEXACOSANE

R.T.: 15.859 min
Delta R.T.: -0.025 min
Response: 2144023
Conc: 13.77 ug/ml

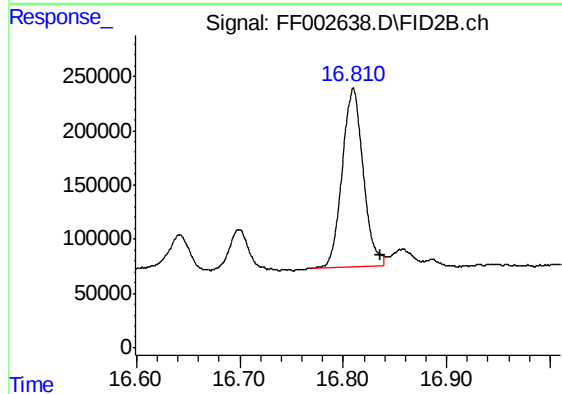

#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: -0.026 min
Response: 2336401
Conc: 15.06 ug/ml m