

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111022\
 Data File : FF011606.D
 Signal(s) : FID2B.ch
 Acq On : 10 Nov 2022 11:42
 Operator : YP\AJ
 Sample : PP21001
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PP21001

Integration File: Sample.e
 Quant Time: Nov 11 05:34:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2)	N-DECANE	4.602	2596812	19.675 ug/ml
3)	N-DODECANE	6.765	2608993	19.411 ug/ml
4)	N-TETRADECANE	8.593	2587460	19.120 ug/ml
5)	N-HEXADECANE	10.200	2605772	18.954 ug/ml
6)	N-OCTADECANE	11.644	2604115	18.826 ug/ml
7)	N-EICOSANE	12.955	2516559	18.196 ug/ml
8)	N-DOCOSANE	14.154	2445893	18.121 ug/ml
10)	N-TETRACOSANE	15.258	2413974	17.801 ug/ml
11)	N-HEXACOSANE	16.280	2317458	17.346 ug/ml
12)	N-OCTACOSANE	17.230	2251464	16.995 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111022\
Data File : FF011606.D
Signal(s) : FID2B.ch
Acq On : 10 Nov 2022 11:42
Operator : YP\AJ
Sample : PP21001
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PP21001

Integration File: Sample.e
Quant Time: Nov 11 05:34:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

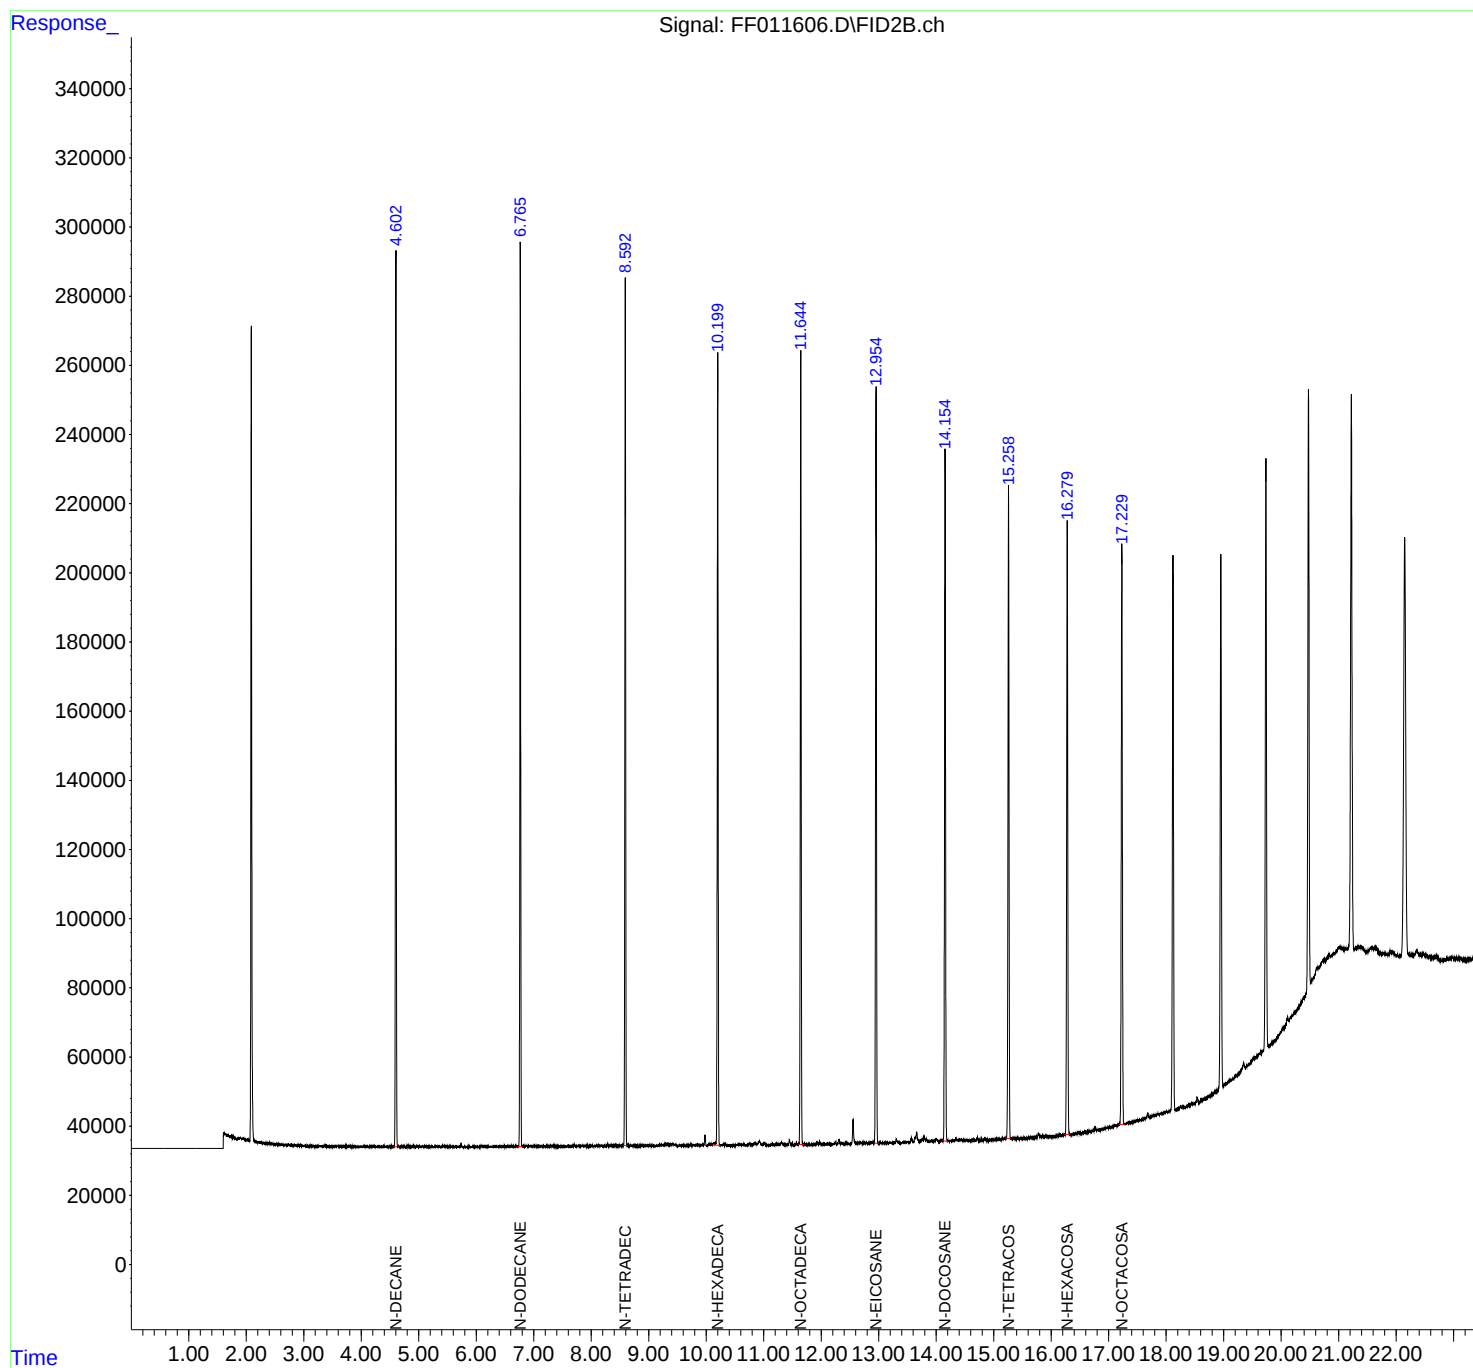


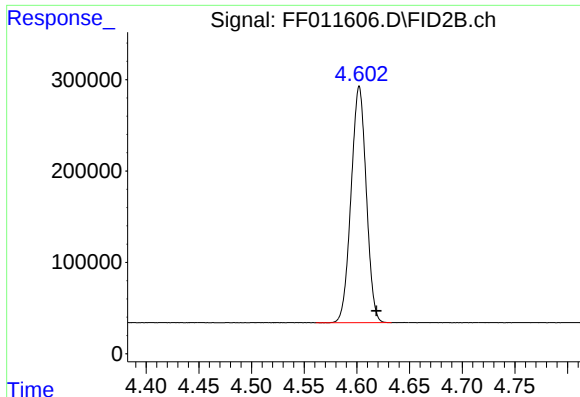

#2 N-DECANE


R.T.: 4.602 min
Delta R.T.: -0.016 min
Response: 2596812
Conc: 19.68 ug/ml

Instrument :
FID_F
ClientSampleId :
PP21001

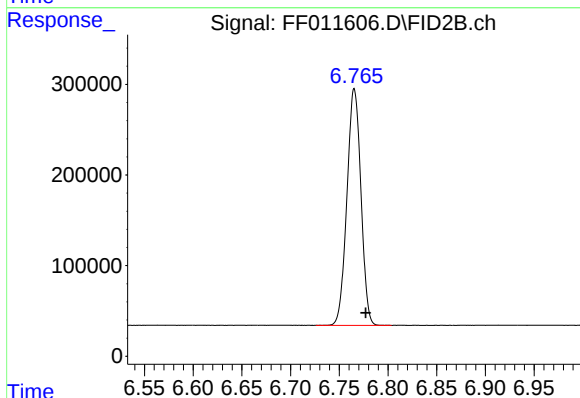


#3 N-DODECANE

R.T.: 6.765 min
Delta R.T.: -0.012 min
Response: 2608993
Conc: 19.41 ug/ml

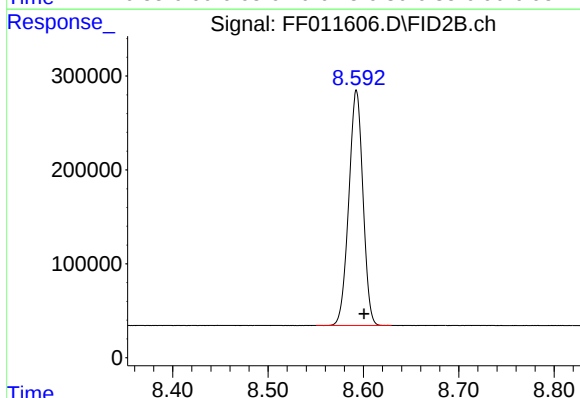


#4 N-TETRADECANE

R.T.: 8.593 min
Delta R.T.: -0.008 min
Response: 2587460
Conc: 19.12 ug/ml

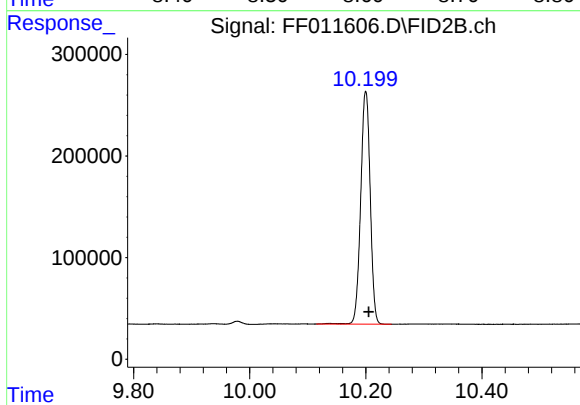

#5 N-HEXADECANE


R.T.: 10.200 min
Delta R.T.: -0.005 min
Response: 2605772
Conc: 18.95 ug/ml

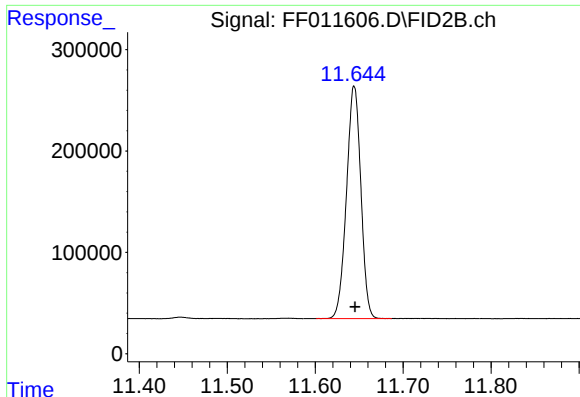

#6 N-OCTADECANE


R.T.: 11.644 min
Delta R.T.: 0.000 min
Response: 2604115
Conc: 18.83 ug/ml

Instrument :
FID_F
ClientSampleId :
PP21001

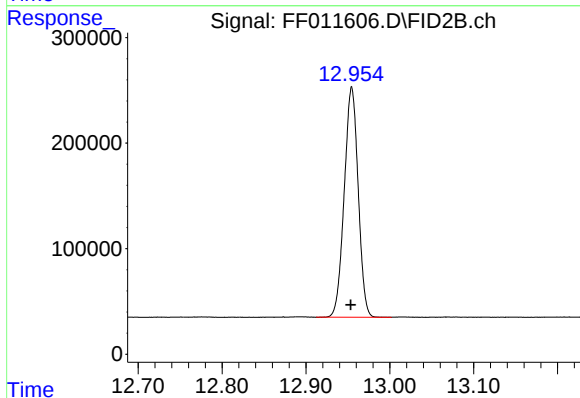


#7 N-EICOSANE

R.T.: 12.955 min
Delta R.T.: 0.001 min
Response: 2516559
Conc: 18.20 ug/ml

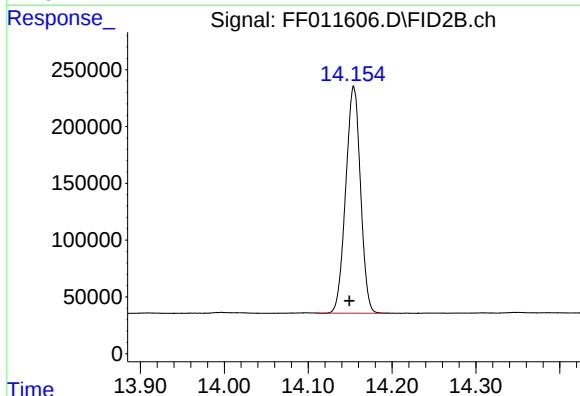


#8 N-DOCOSANE

R.T.: 14.154 min
Delta R.T.: 0.005 min
Response: 2445893
Conc: 18.12 ug/ml

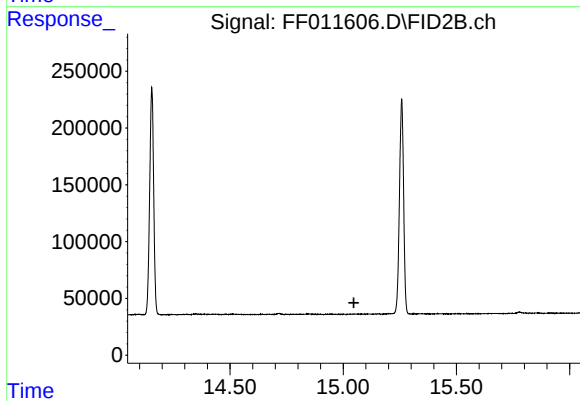

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T. : 15.047 min
Response: 0
Conc: N.D.

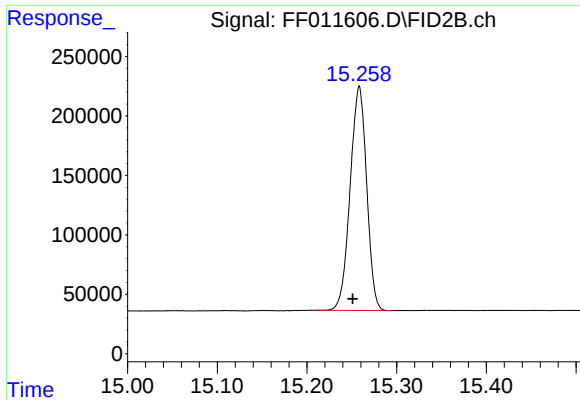

#10 N-TETRACOSANE


R.T.: 15.258 min
Delta R.T.: 0.007 min
Response: 2413974
Conc: 17.80 ug/ml

Instrument :
FID_F
ClientSampleId :
PP21001

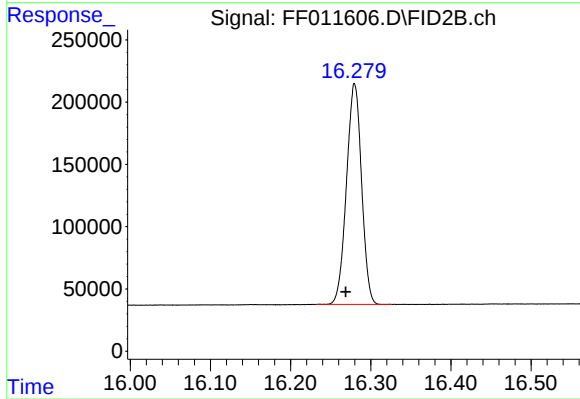

#11 N-HEXACOSANE

R.T.: 16.280 min
Delta R.T.: 0.011 min
Response: 2317458
Conc: 17.35 ug/ml

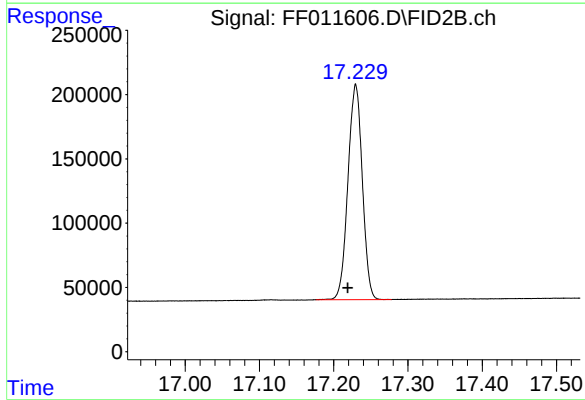

#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: 0.011 min
Response: 2251464
Conc: 16.99 ug/ml