

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111022\
 Data File : FF011610.D
 Signal(s) : FID2B.ch
 Acq On : 10 Nov 2022 16:32
 Operator : YP\AJ
 Sample : PB148949BS
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB148949BS

Integration File: Sample.e
 Quant Time: Nov 11 05:34:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
 Quant Title :
 QLast Update : Fri Nov 04 14:11:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	2150397	18.125 ug/ml
Target Compounds			
2) N-DECANE	4.613	2473418	18.740 ug/ml
3) N-DODECANE	6.774	2516157	18.721 ug/ml
4) N-TETRADECANE	8.599	2523441	18.647 ug/ml
5) N-HEXADECANE	10.205	2545213	18.514 ug/ml
6) N-OCTADECANE	11.647	2546589	18.410 ug/ml
7) N-EICOSANE	12.957	2463154	17.810 ug/ml
8) N-DOCOSANE	14.155	2398436	17.769 ug/ml
10) N-TETRACOSANE	15.258	2352296	17.346 ug/ml
11) N-HEXACOSANE	16.280	2276796	17.041 ug/ml
12) N-OCTACOSANE	17.230	2203195	16.630 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111022\
Data File : FF011610.D
Signal(s) : FID2B.ch
Acq On : 10 Nov 2022 16:32
Operator : YP\AJ
Sample : PB148949BS
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB148949BS

Integration File: Sample.e
Quant Time: Nov 11 05:34:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110422.M
Quant Title :
QLast Update : Fri Nov 04 14:11:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

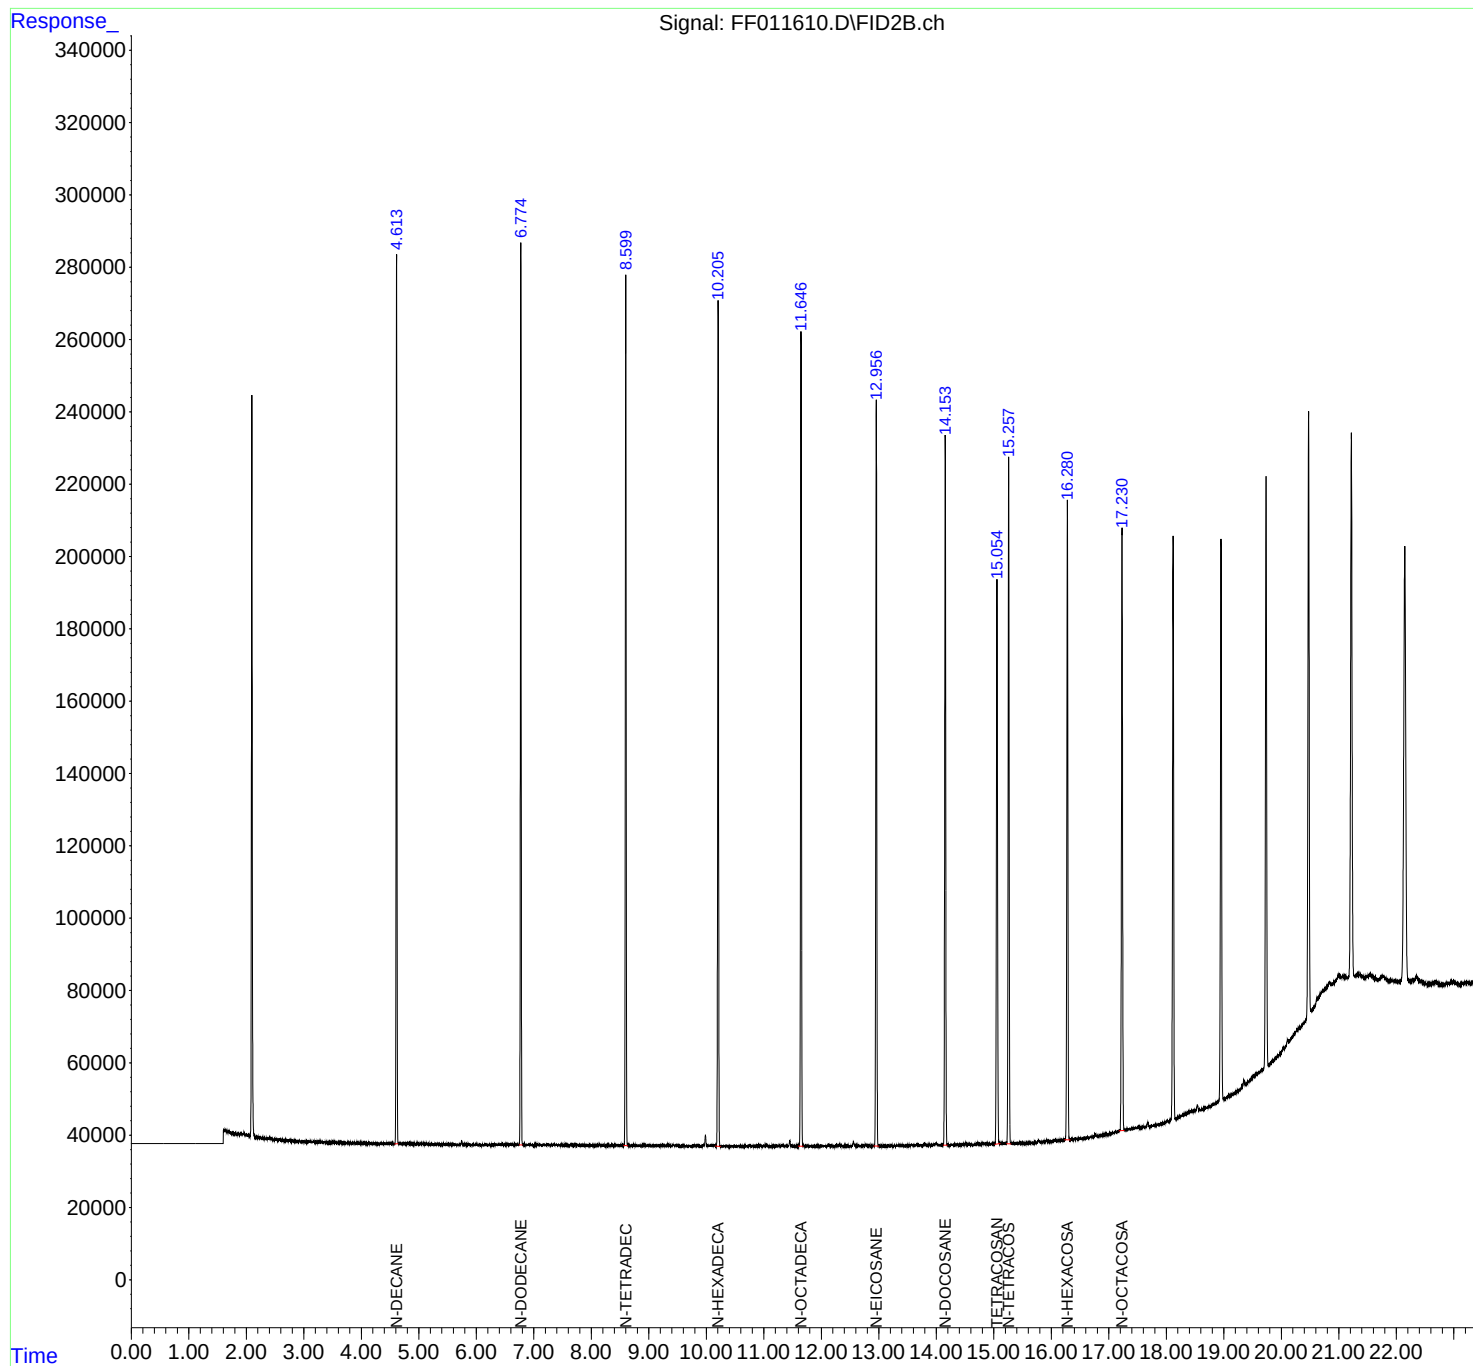


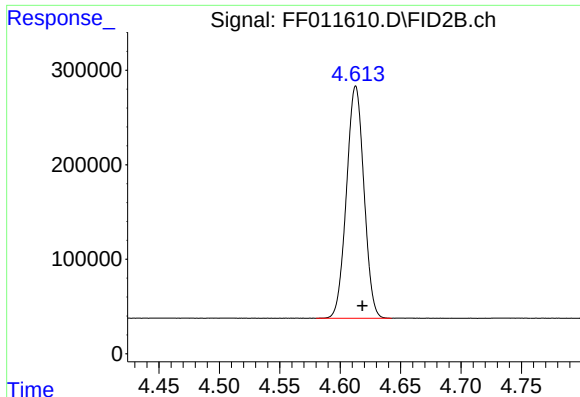

#2 N-DECANE


R.T.: 4.613 min
Delta R.T.: -0.005 min
Response: 2473418
Conc: 18.74 ug/ml

Instrument :
FID_F
ClientSampleId :
PB148949BS

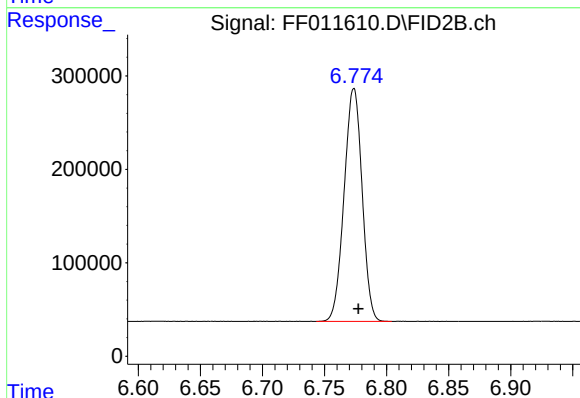


#3 N-DODECANE

R.T.: 6.774 min
Delta R.T.: -0.004 min
Response: 2516157
Conc: 18.72 ug/ml

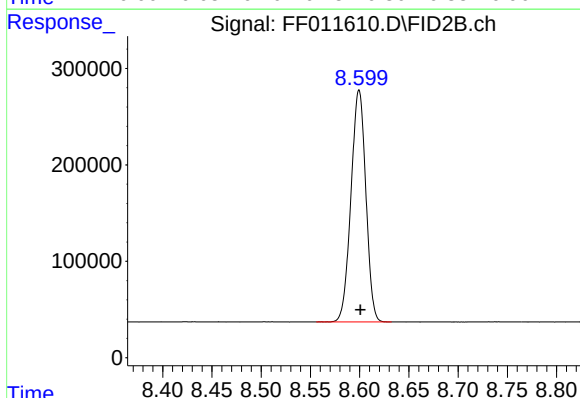


#4 N-TETRADECANE

R.T.: 8.599 min
Delta R.T.: -0.001 min
Response: 2523441
Conc: 18.65 ug/ml

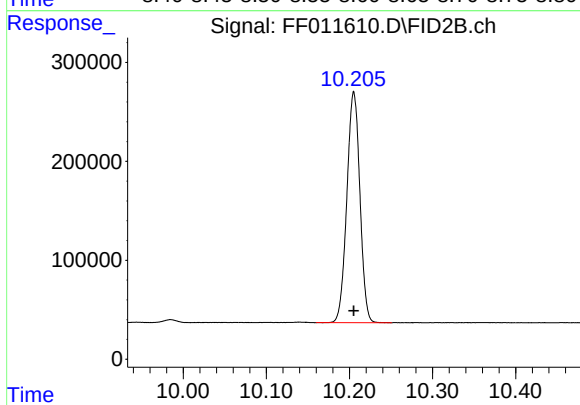

#5 N-HEXADECANE


R.T.: 10.205 min
Delta R.T.: 0.000 min
Response: 2545213
Conc: 18.51 ug/ml

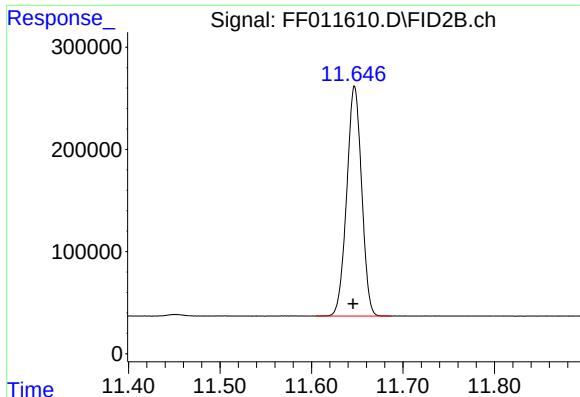

#6 N-OCTADECANE


R.T.: 11.647 min
Delta R.T.: 0.002 min
Response: 2546589
Conc: 18.41 ug/ml

Instrument :
FID_F
ClientSampleId :
PB148949BS

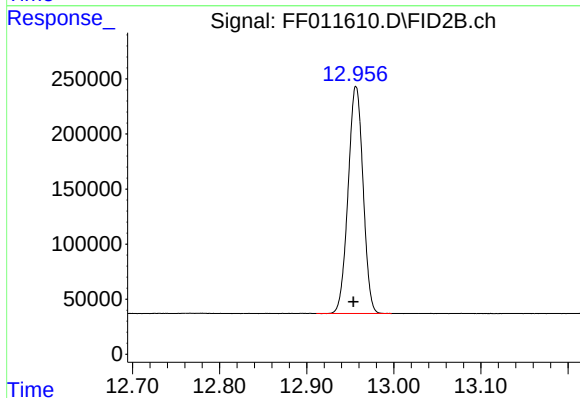


#7 N-EICOSANE

R.T.: 12.957 min
Delta R.T.: 0.003 min
Response: 2463154
Conc: 17.81 ug/ml

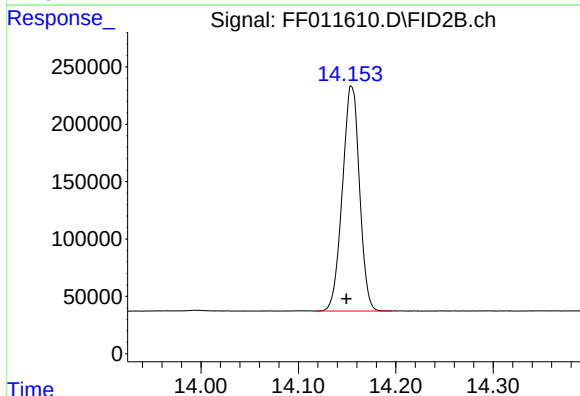


#8 N-DOCOSANE

R.T.: 14.155 min
Delta R.T.: 0.005 min
Response: 2398436
Conc: 17.77 ug/ml

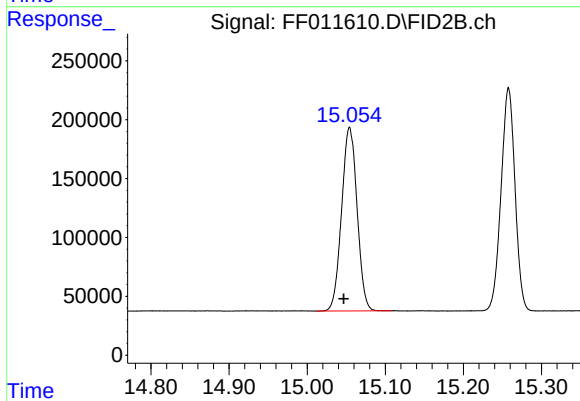

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.054 min
Delta R.T.: 0.007 min
Response: 2150397
Conc: 18.12 ug/ml

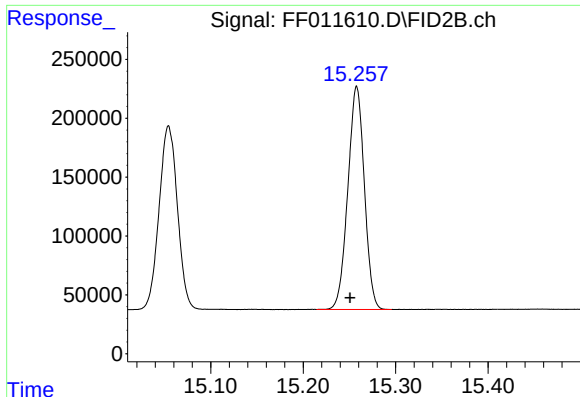

#10 N-TETRACOSANE


R.T.: 15.258 min
Delta R.T.: 0.007 min
Response: 2352296
Conc: 17.35 ug/ml

Instrument :
FID_F
ClientSampleId :
PB148949BS

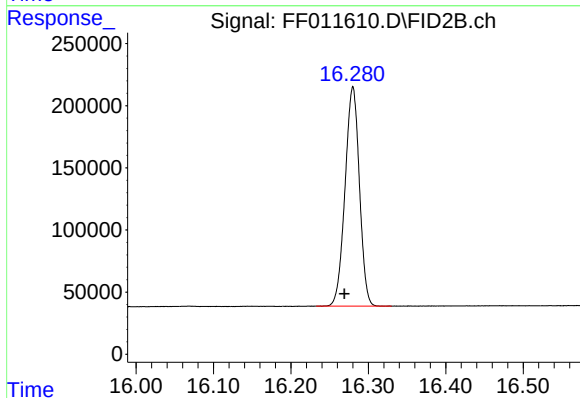

#11 N-HEXACOSANE

R.T.: 16.280 min
Delta R.T.: 0.011 min
Response: 2276796
Conc: 17.04 ug/ml

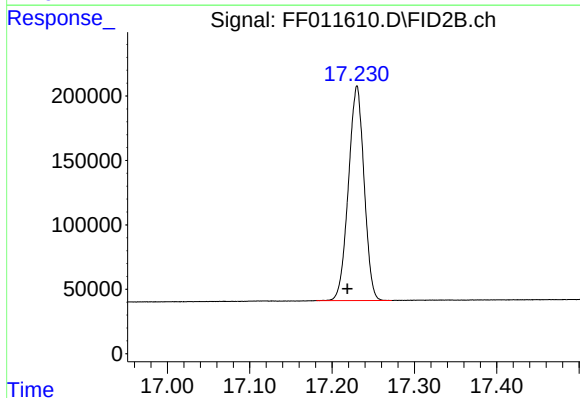

#12 N-OCTACOSANE

R.T.: 17.230 min
Delta R.T.: 0.012 min
Response: 2203195
Conc: 16.63 ug/ml